

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
 Data File : BM034865.D
 Acq On : 28 Apr 2022 14:02
 Operator : CG/JU
 Sample : PB144441BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB144441BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.505	404	411	421	rBV	4687023	6555110	70.33%	12.733%
2	7.093	673	681	692	rBV	4177920	6642863	71.27%	12.903%
3	7.928	817	823	832	rVB	819049	1305111	14.00%	2.535%
4	9.087	1012	1020	1031	rBV	2611136	4257523	45.68%	8.270%
5	10.734	1292	1300	1308	rBV	1037995	1698435	18.22%	3.299%
6	13.192	1710	1718	1725	rBV	6410972	8997170	96.53%	17.476%
7	14.563	1944	1951	1962	rBV	1398892	1997414	21.43%	3.880%
8	16.045	2196	2203	2218	rBV	4040969	5477327	58.77%	10.639%
9	17.304	2410	2417	2424	rVB	1433970	2031731	21.80%	3.947%
10	19.927	2857	2863	2868	rBV	7735566	9320314	100.00%	18.104%
11	21.480	3122	3127	3133	rBV	1309937	1685393	18.08%	3.274%
12	23.868	3527	3533	3541	rVB2	780767	1513260	16.24%	2.939%




Sum of corrected areas: 51481651

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034865.D
Acq On : 28 Apr 2022 14:02
Operator : CG/JU
Sample : PB144441BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144441BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

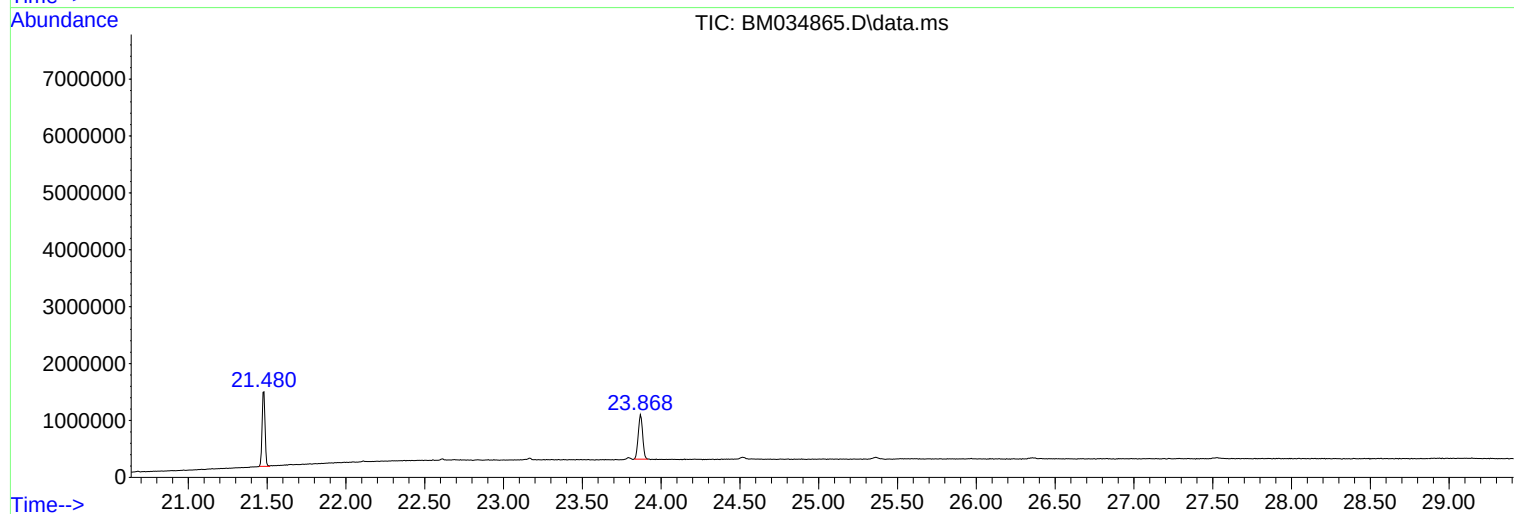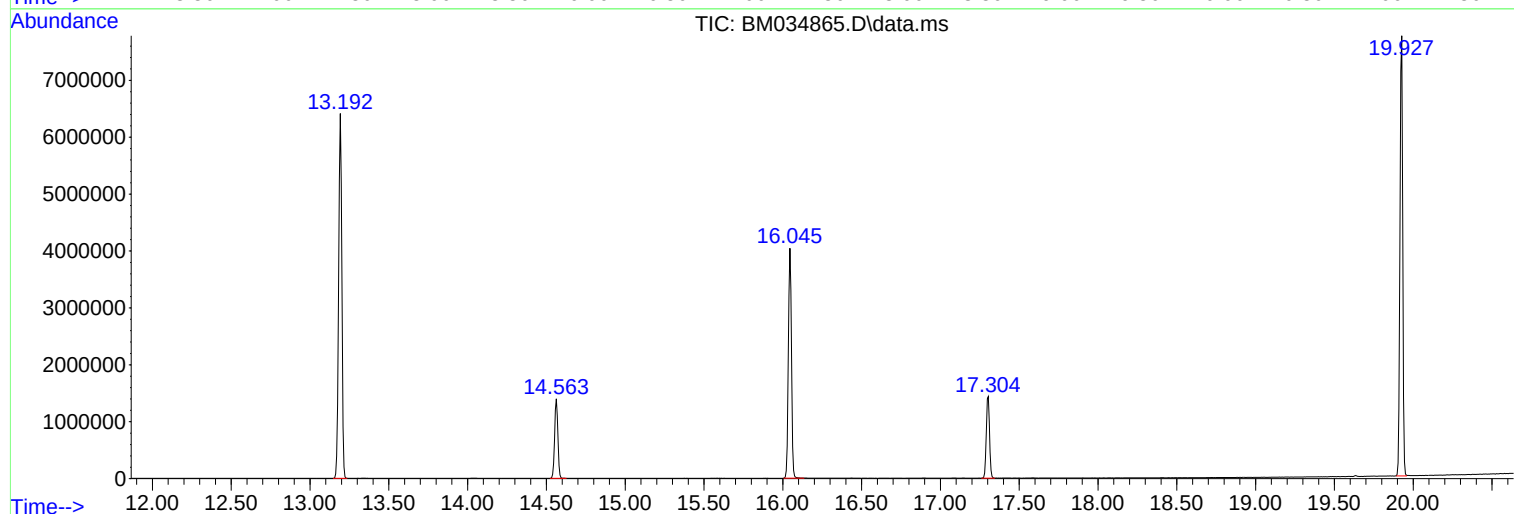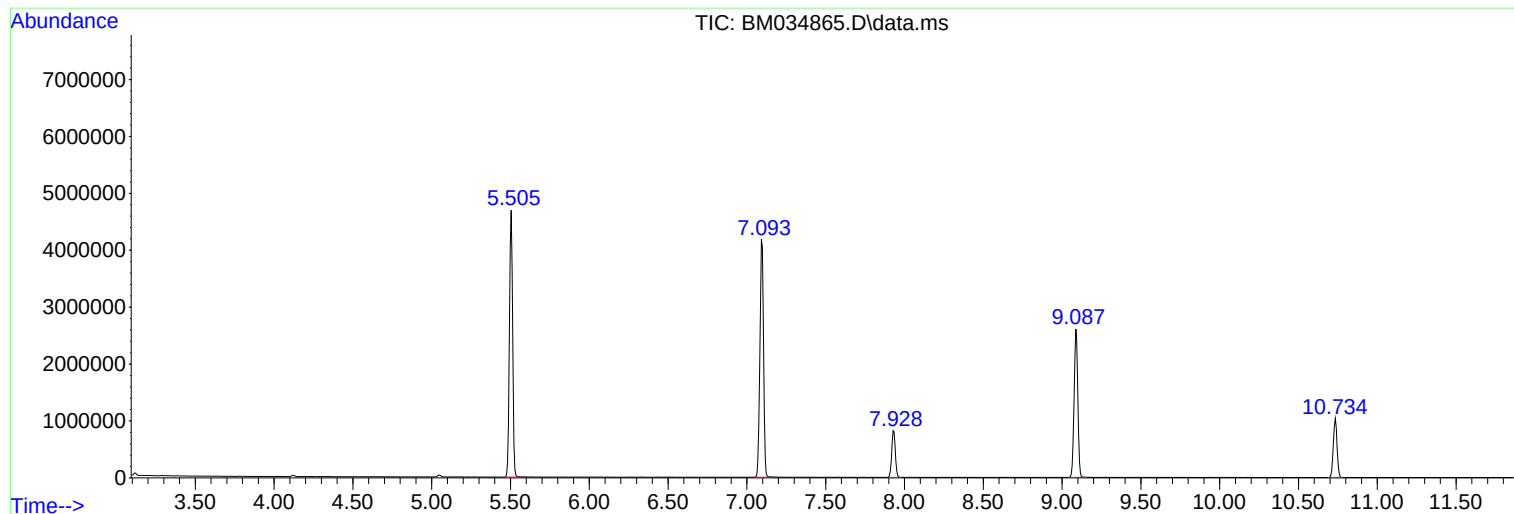

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034865.D
Acq On : 28 Apr 2022 14:02
Operator : CG/JU
Sample : PB144441BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144441BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034865.D
Acq On : 28 Apr 2022 14:02
Operator : CG/JU
Sample : PB144441BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144441BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------