
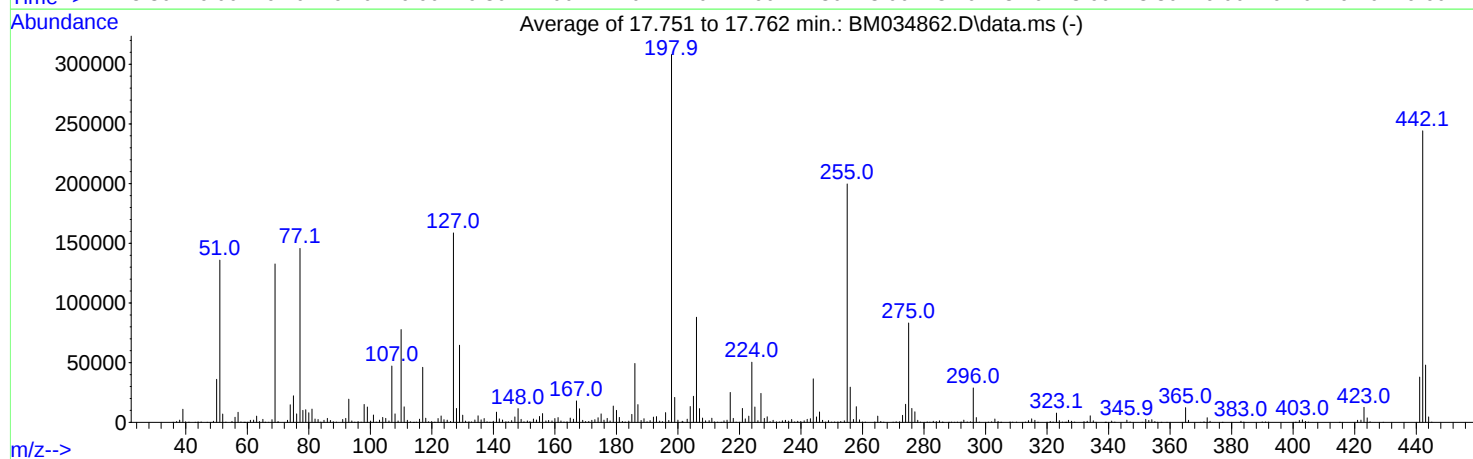


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
 Data File : BM034862.D
 Acq On : 28 Apr 2022 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 01:51:59 2022

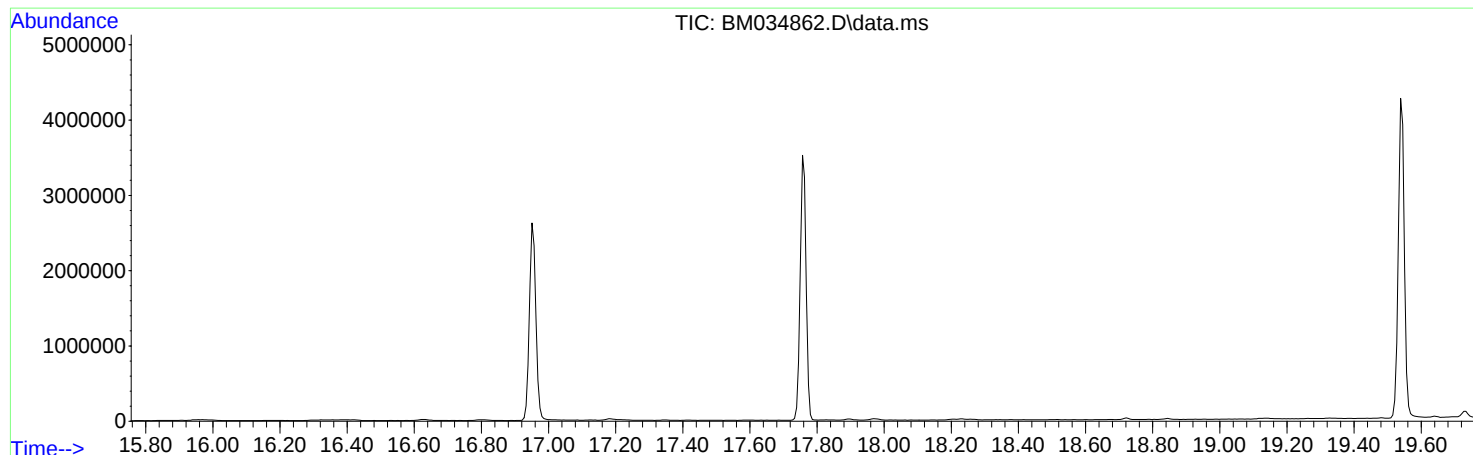




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	135939	PASS
68	69	0.00	2	1.7	2250	PASS
69	198	0.00	100	43.1	132691	PASS
70	69	0.00	2	0.4	586	PASS
127	198	10	80	51.5	158693	PASS
197	198	0.00	2	0.5	1590	PASS
198	198	100	100	100.0	308160	PASS
199	198	5	9	6.8	20964	PASS
275	198	10	60	27.0	83187	PASS
365	198	1	100	4.0	12350	PASS
441	198	0.01	100	12.3	37909	PASS
442	442	50	100	100.0	244184	PASS
443	442	15	24	19.6	47968	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
 Data File : BM034862.D
 Acq On : 28 Apr 2022 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 29 06:04:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 01:51:59 2022
 Response via : Initial Calibration

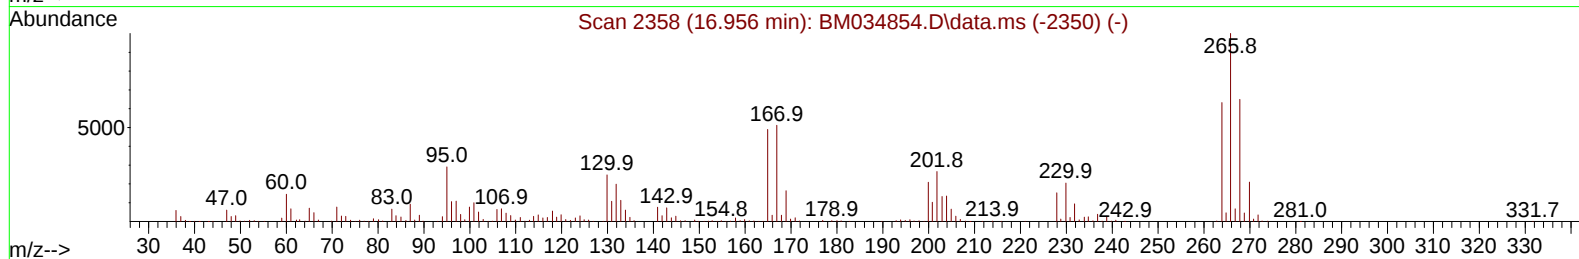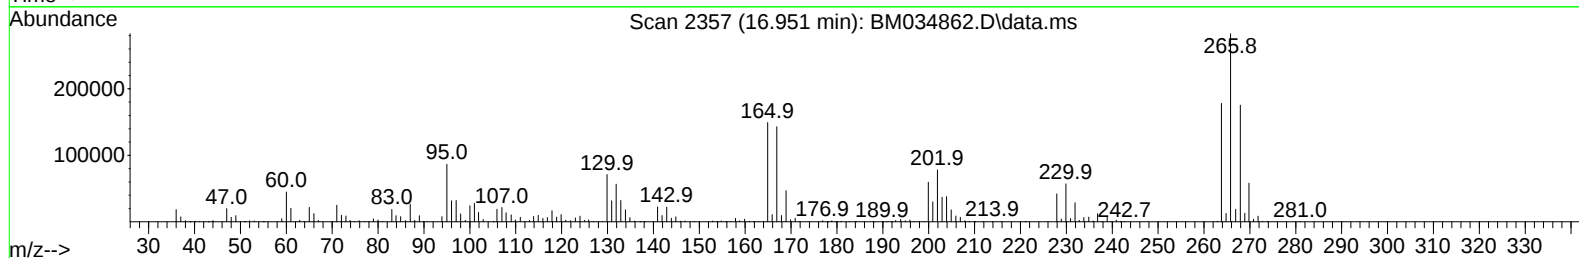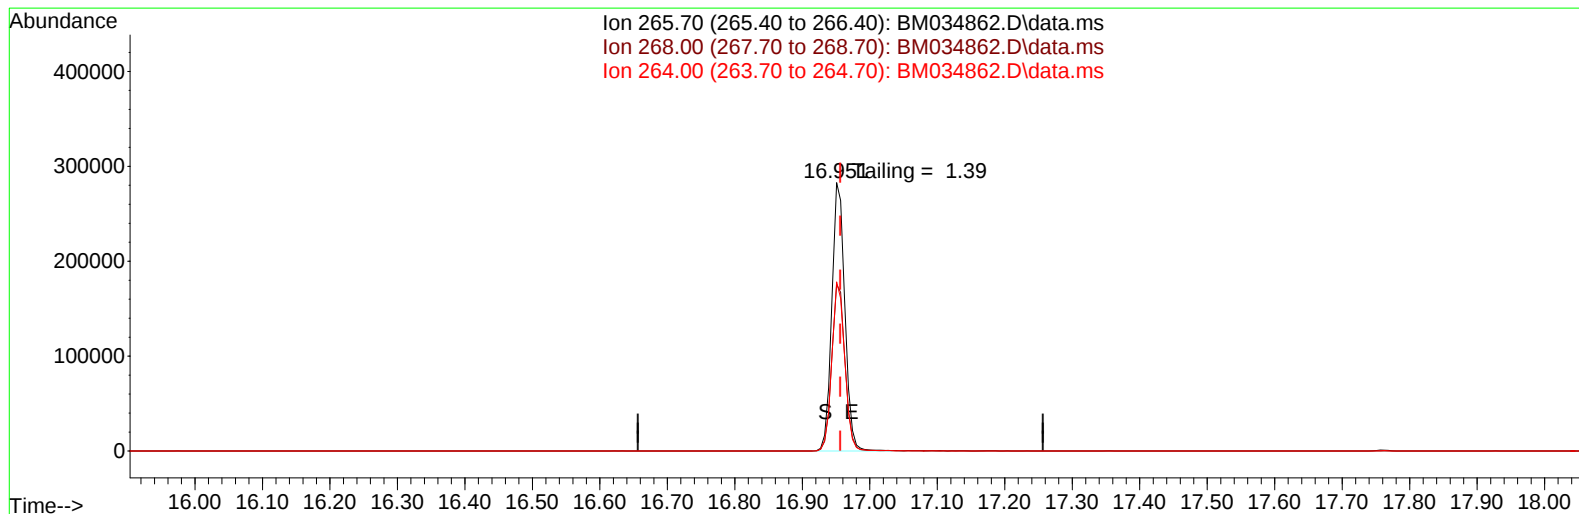

TIC: BM034862.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.006) 980155.90 ng




response 380586

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.10
264.00	63.30	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034862.D
Acq On : 28 Apr 2022 12:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 29 06:04:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration

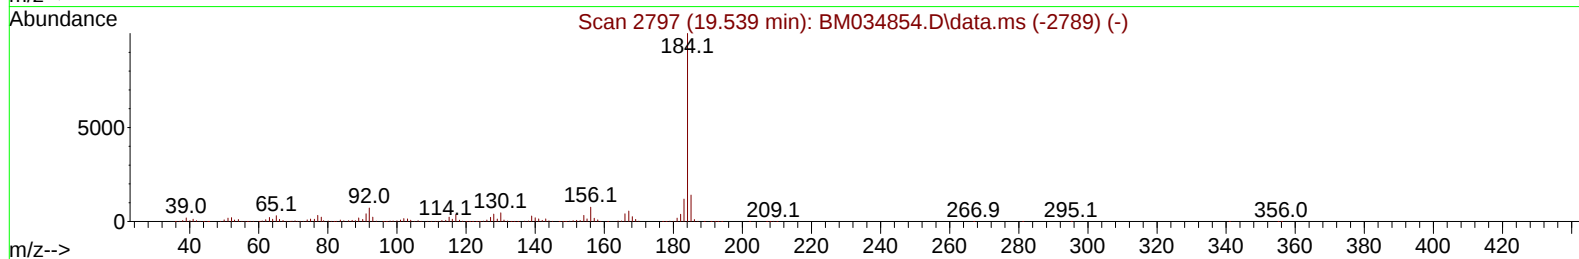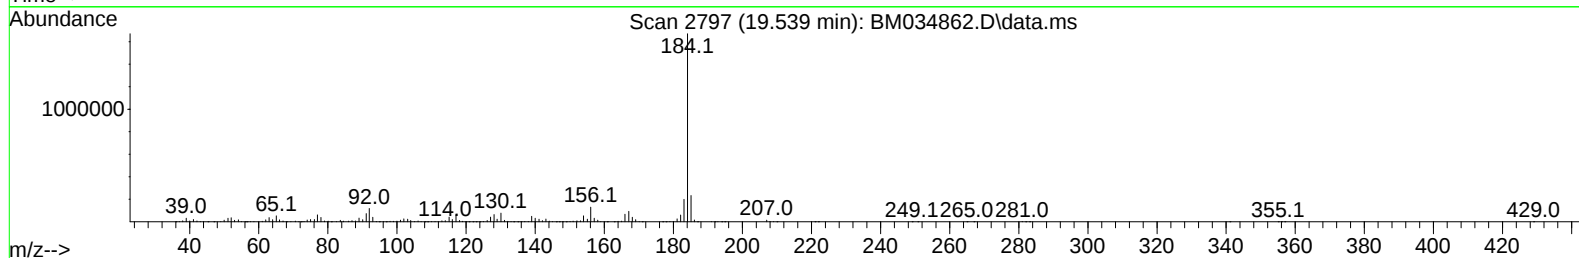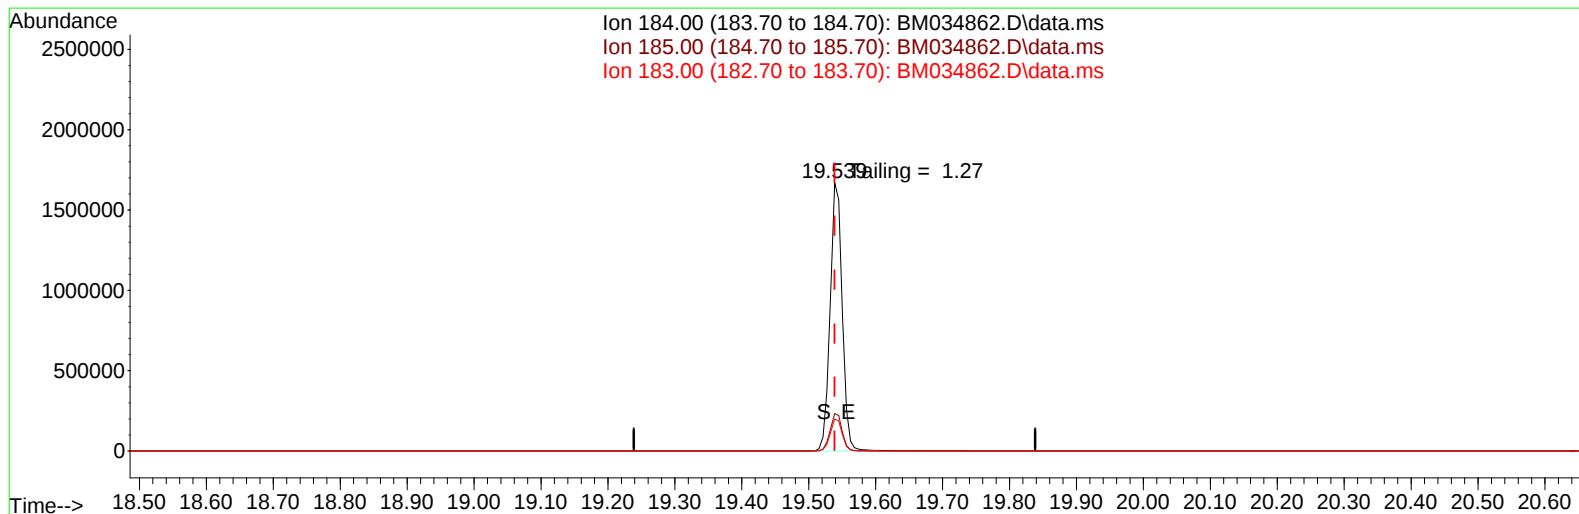

TIC: BM034862.D\data.ms

(77) Benzidine

19.539min (+ 0.000) 20256.51 ng

response 2102761

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.99
183.00	11.90	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/28/2022	BNA_M	<u>BM034862.D</u>
Compound Name	Response	Retention Time
DDT	1043494	20.786
DDD	6034	20.398
DDE	400	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6434	1049928	0.61

Instrument :
BNA_M
ClientSampleId :
DFTPP