


Data Path : Z:\HPCHEM1\BNA_M\Data\BM042915\
 Data File : BM001131.D
 Acq On : 28 Apr 2015 16:22
 Operator : TP/IZ
 Sample : DFTPP52
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP53

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 28 06:36:34 2015

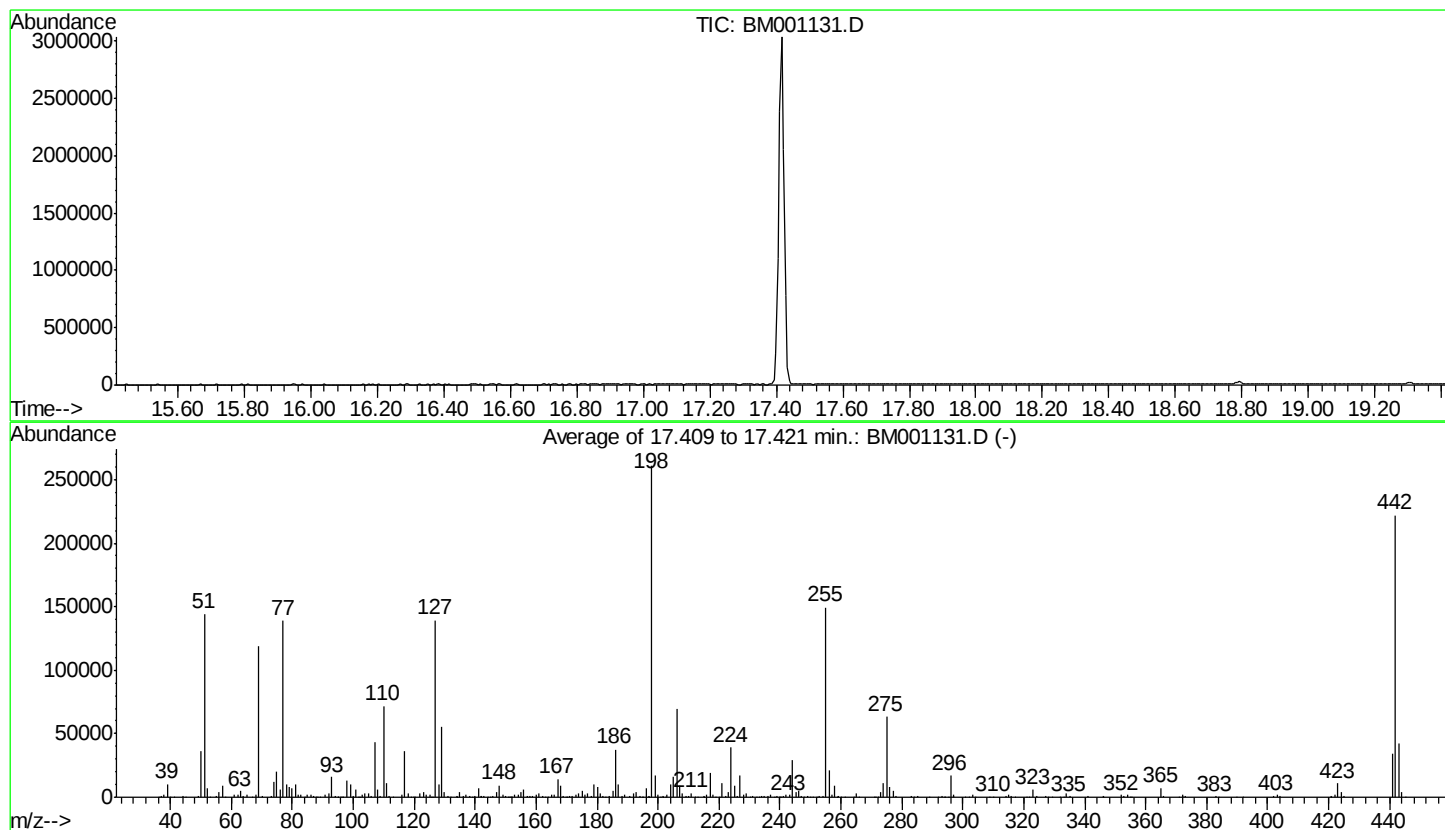

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	144138	PASS
68	69	0.00	2	1.6	1942	PASS
69	198	0.00	100	45.5	118818	PASS
70	69	0.00	2	0.6	658	PASS
127	198	10	80	53.4	139373	PASS
197	198	0.00	2	0.3	669	PASS
198	198	100	100	100.0	261013	PASS
199	198	5	9	6.5	16901	PASS
275	198	10	60	24.2	63184	PASS
365	198	1	100	2.8	7203	PASS
441	443	0.01	100	81.0	34693	PASS
442	198	50	100	85.1	222122	PASS
443	442	15	24	19.3	42832	PASS