


Data Path : Z:\HPCHEM1\BNA_M\Data\BM042916\
 Data File : BM005134.D
 Acq On : 29 Apr 2016 08:39
 Operator : UM/SJ
 Sample : DFTPP60
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP60

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM041816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 29 13:46:03 2016

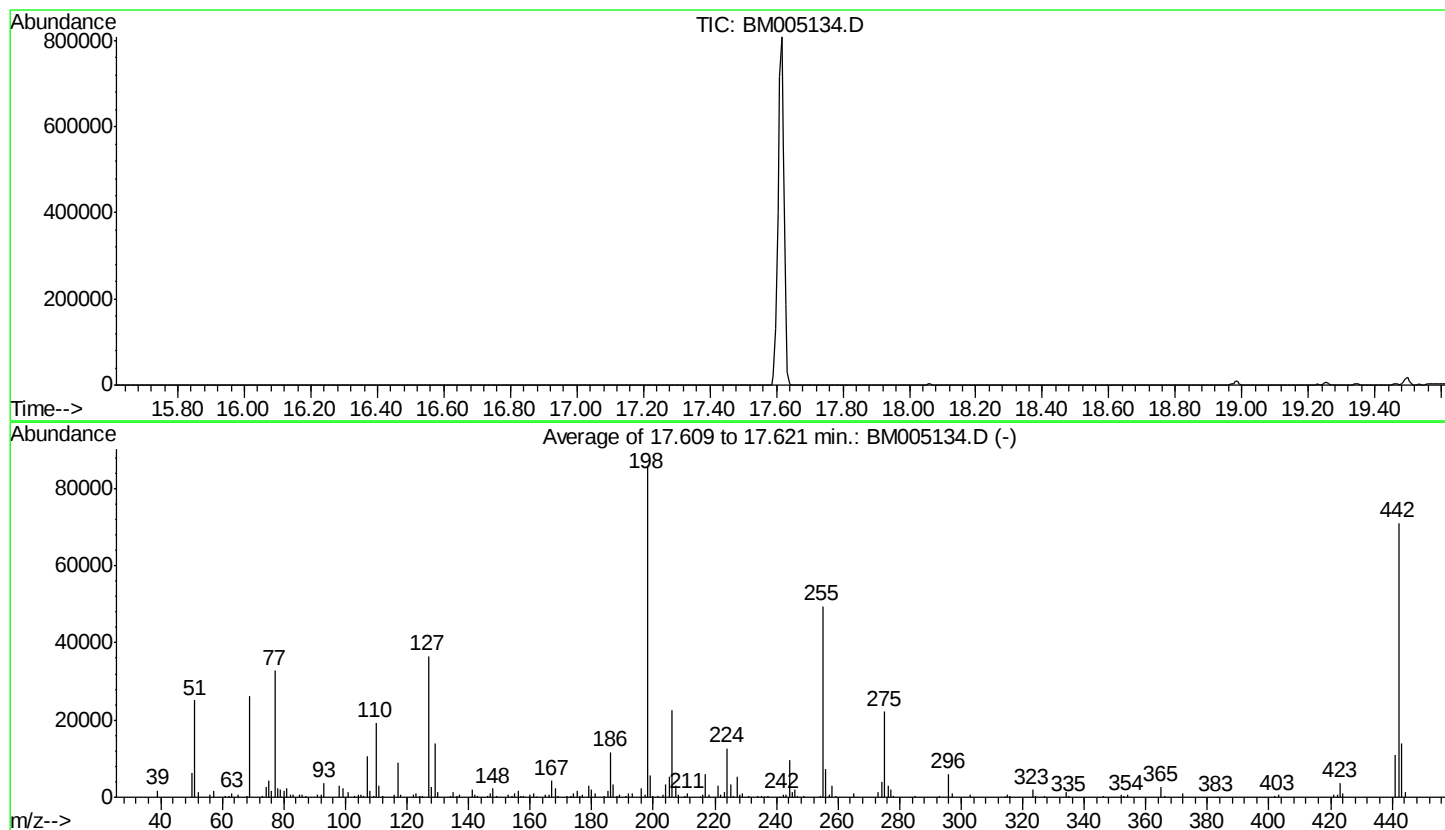

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	25133	PASS
68	69	0.00	2	1.7	447	PASS
69	198	0.00	100	30.6	26317	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.5	36552	PASS
197	198	0.00	2	0.7	579	PASS
198	198	100	100	100.0	85909	PASS
199	198	5	9	6.7	5734	PASS
275	198	10	60	25.7	22109	PASS
365	198	1	100	3.3	2794	PASS
441	443	0.01	100	79.3	10922	PASS
442	198	50	100	82.7	71064	PASS
443	442	15	24	19.4	13778	PASS

m/z	Abundance
39.10	2049.0
50.10	7224.0
51.10	29272.0
52.10	1487.0
56.00	808.0
57.00	2014.0
61.10	344.0
62.00	450.0
63.00	1237.0
65.00	629.0
68.00	530.0
69.00	29792.0
73.10	321.0
74.10	3221.0
75.00	5050.0
76.10	1763.0
77.10	37376.0
78.10	2639.0
79.00	2356.0
80.00	1765.0
81.00	2519.0
82.00	662.0
83.00	631.0
85.00	549.0
86.00	738.0
87.00	343.0
91.00	585.0
92.00	608.0
93.00	4337.0
98.00	3523.0
99.00	2756.0
101.00	1474.0
103.00	498.0
104.00	998.0
105.00	898.0
106.00	315.0
107.00	11974.0
108.00	1942.0
109.10	362.0
110.00	21600.0
111.00	3336.0
112.00	431.0
116.00	617.0
117.00	9919.0
118.00	802.0
122.00	872.0
123.00	1177.0
124.00	529.0
125.00	483.0
127.00	40408.0
128.00	2999.0
129.00	15062.0
130.00	1377.0
134.00	427.0
135.00	1259.0
136.00	529.0
137.10	722.0
141.00	2087.0
142.00	729.0
143.00	457.0
146.00	396.0
147.00	1129.0
148.00	2596.0
149.00	566.0
153.00	632.0
154.00	527.0
155.00	1232.0
156.10	1671.0
157.00	342.0
157.90	362.0
160.00	725.0
161.00	1010.0
165.00	760.0
166.00	682.0
167.10	4465.0
168.00	2543.0
169.00	420.0
171.90	376.0
173.00	487.0
174.00	923.0
175.10	1760.0
176.10	486.0
177.00	783.0
179.00	3349.0
180.00	2296.0
181.00	1023.0
184.00	311.0
185.10	1603.0
186.10	12459.0
187.10	3699.0
188.10	426.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

189.00	756.0
191.00	371.0
192.00	1033.0
193.00	1176.0
196.00	2453.0
197.10	620.0
198.00	89432.0
199.00	6169.0
200.00	500.0
201.60	334.0
203.00	578.0
204.10	3219.0
205.10	5493.0
206.10	23336.0
207.10	3207.0
208.00	710.0
210.20	323.0
211.00	867.0
216.10	520.0
217.00	6064.0
218.00	852.0
221.10	3077.0
221.90	775.0
223.00	1300.0
224.10	13223.0
225.10	3300.0
226.10	415.0
227.10	5170.0
228.00	824.0
229.00	1105.0
231.00	388.0
234.00	322.0
235.00	374.0
237.10	535.0
242.00	659.0
243.10	673.0
244.10	9995.0
245.10	1427.0
246.00	1975.0
246.90	366.0
249.00	322.0
254.20	466.0
255.10	48560.0
256.10	7313.0
257.00	586.0
258.00	2909.0
259.10	496.0
265.00	1133.0
273.00	1438.0
274.00	4023.0
275.10	21792.0
276.10	2941.0
277.00	1833.0
278.00	366.0
285.00	356.0
293.00	444.0
296.00	5739.0
297.00	840.0
303.10	678.0
315.00	594.0
316.00	421.0
323.10	1800.0
324.10	302.0
327.00	424.0
334.10	1227.0
335.00	339.0
346.00	431.0
352.10	565.0
353.00	411.0
354.10	535.0
365.00	2513.0
366.00	397.0
372.10	893.0
402.00	344.0
403.00	532.0
421.10	501.0
422.00	482.0
423.10	3126.0
424.10	1021.0
441.10	8989.0
442.10	59232.0
443.10	12133.0
444.10	1216.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.10	1911.0
50.10	7029.0
51.10	28480.0
52.10	1470.0
56.00	883.0
57.00	1990.0
61.00	381.0
62.00	461.0
63.10	1166.0
65.10	615.0
68.10	502.0
69.00	30712.0
73.00	320.0
74.10	3084.0
75.00	4956.0
76.10	1722.0
77.10	37760.0
78.10	2536.0
79.00	2298.0
80.00	1776.0
81.00	2747.0
82.00	711.0
83.00	697.0
85.00	631.0
86.00	710.0
87.00	365.0
91.00	614.0
92.00	659.0
93.00	4257.0
98.00	3352.0
99.00	2759.0
101.00	1573.0
103.00	516.0
104.00	968.0
105.00	900.0
106.00	327.0
107.00	12174.0
108.00	1815.0
109.10	383.0
110.00	21976.0
111.00	3382.0
112.00	371.0
116.00	695.0
117.00	10239.0
118.00	787.0
122.00	771.0
123.00	1238.0
124.00	540.0
125.00	492.0
127.10	42384.0
128.00	3328.0
129.00	15973.0
130.00	1422.0
134.00	481.0
135.00	1439.0
136.00	567.0
137.00	723.0
141.00	2070.0
142.00	687.0
143.00	530.0
146.00	361.0
147.00	1185.0
148.00	2702.0
149.00	543.0
153.00	766.0
154.00	630.0
155.00	1222.0
156.10	1874.0
157.00	371.0
158.00	466.0
160.00	688.0
161.00	1087.0
162.00	309.0
165.00	862.0
166.00	692.0
167.00	4993.0
168.10	2687.0
169.00	425.0
172.00	444.0
173.10	513.0
174.00	1058.0
175.10	1930.0
176.00	577.0
177.00	786.0
179.00	3540.0
180.00	2455.0
181.00	1121.0
184.00	304.0
185.00	1755.0
186.10	13488.0
187.10	3860.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

188.00	442.0
189.00	924.0
191.00	449.0
192.00	1174.0
193.10	1261.0
196.10	2687.0
197.20	677.0
198.00	100320.0
199.00	6647.0
200.00	531.0
201.50	343.0
203.00	702.0
204.10	3812.0
205.10	6227.0
206.10	26240.0
207.10	3752.0
208.10	951.0
210.10	404.0
211.10	969.0
215.00	348.0
216.00	572.0
217.00	6744.0
218.00	935.0
221.10	3604.0
221.90	883.0
223.10	1570.0
224.10	14620.0
225.10	3753.0
226.10	426.0
227.00	5956.0
228.00	912.0
229.00	1253.0
231.00	531.0
234.00	367.0
235.00	458.0
236.00	311.0
237.00	471.0
241.00	304.0
242.10	764.0
243.00	786.0
244.10	11310.0
245.10	1401.0
246.00	2318.0
247.00	458.0
249.00	436.0
254.20	601.0
255.10	57936.0
256.10	8385.0
257.10	683.0
258.00	3323.0
259.00	528.0
265.00	1409.0
273.10	1799.0
274.00	4791.0
275.10	25800.0
276.10	3450.0
277.00	2308.0
278.00	411.0
285.00	406.0
293.00	531.0
296.10	7332.0
297.00	1084.0
303.10	868.0
314.00	356.0
315.00	787.0
316.00	429.0
323.10	2312.0
324.10	427.0
327.00	445.0
334.10	1435.0
335.00	335.0
346.00	533.0
352.10	684.0
353.00	407.0
354.00	769.0
365.00	3245.0
366.00	428.0
372.10	1239.0
383.00	362.0
402.00	481.0
403.10	610.0
421.10	655.0
422.10	709.0
423.10	4268.0
424.10	1206.0
441.10	12908.0
442.10	83808.0
443.10	16113.0
444.10	1568.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	1117.0
50.10	4252.0
51.10	17648.0
52.00	916.0
56.00	547.0
57.00	1205.0
63.00	699.0
65.00	380.0
68.10	310.0
69.00	18448.0
73.00	300.0
74.00	1951.0
75.00	3044.0
76.10	1131.0
77.10	23056.0
78.10	1467.0
79.00	1476.0
80.00	1098.0
81.00	1621.0
82.00	448.0
83.00	364.0
85.00	408.0
86.00	477.0
91.00	420.0
92.00	429.0
93.00	2690.0
98.00	2147.0
99.00	1619.0
101.00	946.0
103.00	346.0
104.00	532.0
105.00	663.0
107.00	7659.0
108.00	1198.0
110.00	14147.0
111.00	2189.0
116.00	443.0
117.00	6452.0
118.00	503.0
122.00	576.0
123.00	806.0
124.00	317.0
125.00	342.0
127.00	26864.0
128.10	1945.0
129.00	10296.0
130.00	800.0
135.00	917.0
136.00	323.0
137.00	512.0
141.00	1428.0
142.00	455.0
147.00	727.0
148.00	1656.0
149.00	367.0
153.00	488.0
154.00	341.0
155.00	796.0
156.00	1356.0
160.00	461.0
161.00	720.0
165.00	589.0
166.00	401.0
167.00	3324.0
168.00	1859.0
173.00	368.0
174.00	691.0
175.10	1253.0
176.00	346.0
177.00	577.0
179.00	2385.0
180.10	1651.0
181.00	793.0
185.10	1231.0
186.10	9390.0
187.10	2421.0
189.00	584.0
191.00	328.0
192.00	708.0
193.00	926.0
196.00	1949.0
197.10	441.0
198.00	67976.0
199.00	4388.0
200.00	391.0
203.00	511.0
204.10	2468.0
205.10	4242.0
206.10	18360.0
207.10	2368.0
208.00	635.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

211.00	709.0
216.00	433.0
217.00	4968.0
218.00	629.0
221.10	2609.0
221.90	606.0
223.00	1064.0
224.10	10015.0
225.10	2717.0
227.00	4360.0
228.00	623.0
229.00	900.0
231.00	328.0
237.00	396.0
242.10	581.0
243.10	516.0
244.10	7930.0
245.10	1048.0
246.00	1570.0
247.00	312.0
248.90	310.0
254.20	437.0
255.10	42024.0
256.10	6064.0
257.00	518.0
258.00	2504.0
259.00	383.0
265.00	927.0
273.00	1185.0
274.10	3560.0
275.10	18736.0
276.10	2466.0
277.00	1697.0
278.10	306.0
293.00	415.0
296.00	5320.0
297.00	711.0
303.10	644.0
315.00	621.0
316.00	336.0
323.10	1863.0
324.10	330.0
327.00	339.0
334.10	1199.0
346.00	399.0
352.00	508.0
353.00	370.0
354.10	589.0
365.00	2625.0
366.00	351.0
372.10	1021.0
402.00	335.0
403.10	552.0
421.00	451.0
422.00	499.0
423.10	3794.0
424.10	864.0
441.10	10870.0
442.10	70152.0
443.10	13090.0
444.10	1231.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

Scan 2533 (17.586 min): BM005134.D
DFTPP60

m/z	Abundance
77.00	359.0
198.00	447.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60