
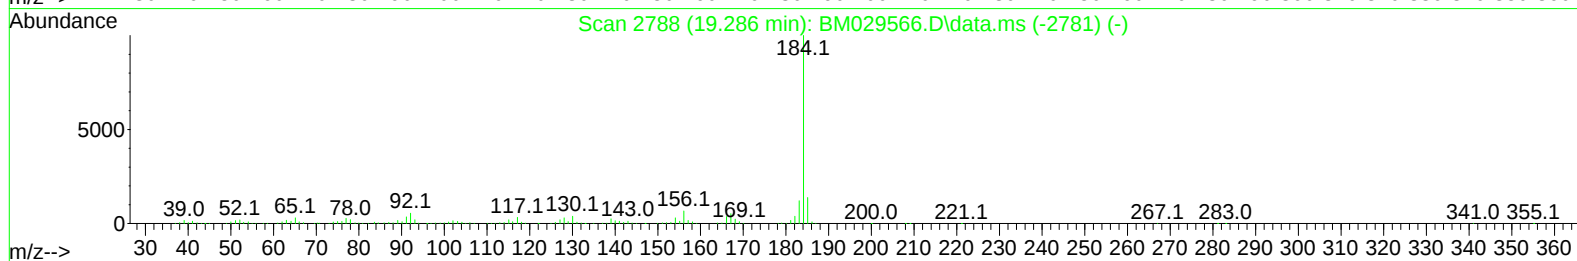
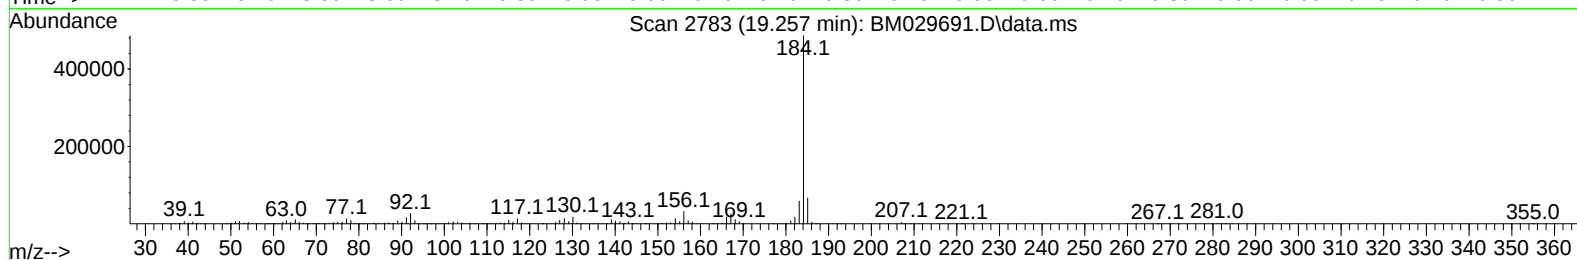


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042921\
 Data File : BM029691.D
 Acq On : 28 Apr 2021 16:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 16:46:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 28 09:28:15 2021
 Response via : Initial Calibration

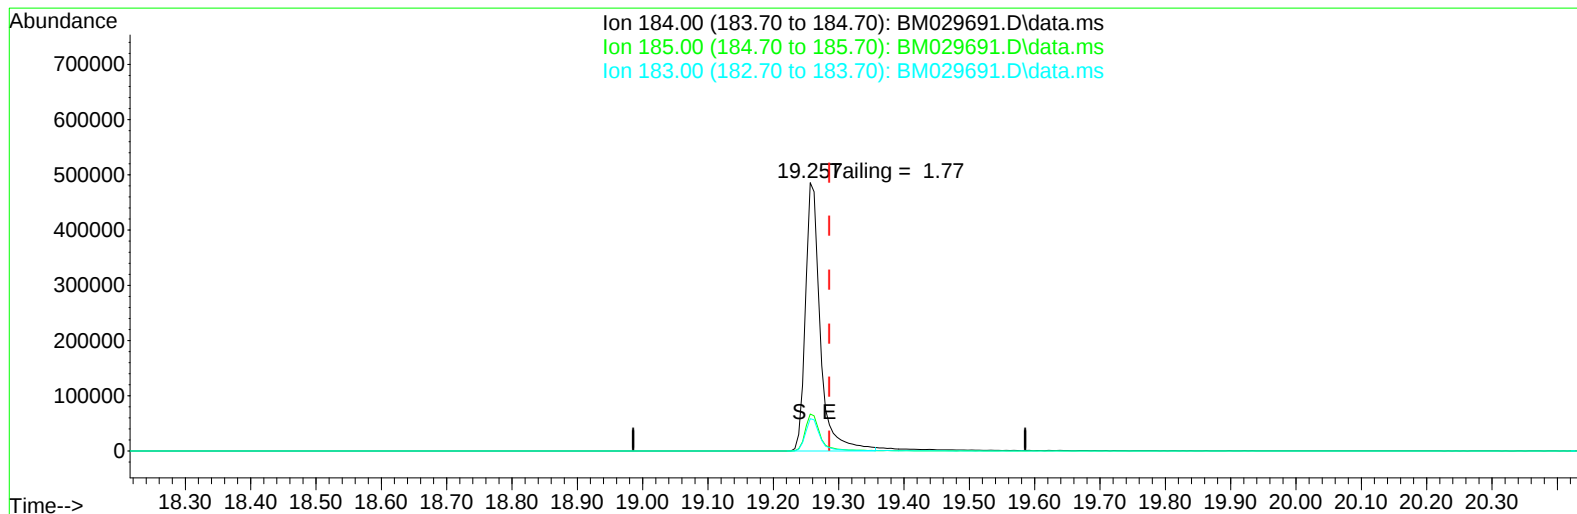




TIC: BM029691.D\data.ms

(77) Benzidine**19.257min (-0.029) 175451.73 ng****response 787521**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.77
183.00	12.30	12.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042921\
Data File : BM029691.D
Acq On : 28 Apr 2021 16:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 16:46:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 28 09:28:15 2021
Response via : Initial Calibration

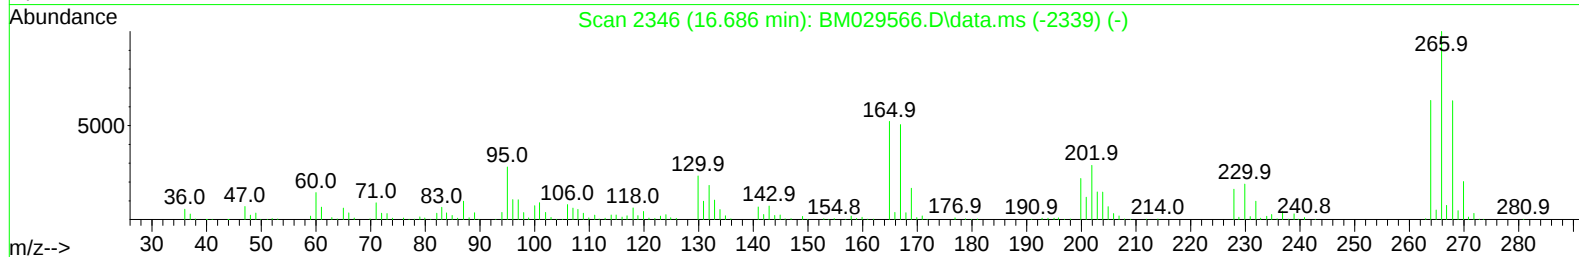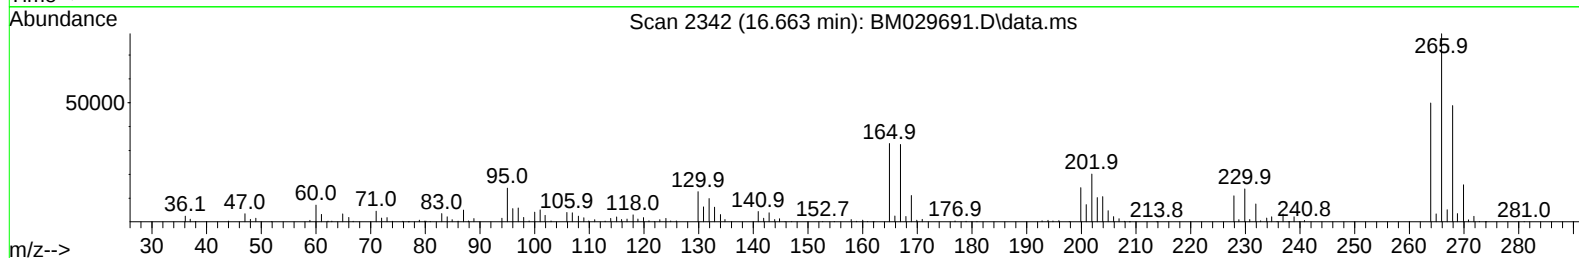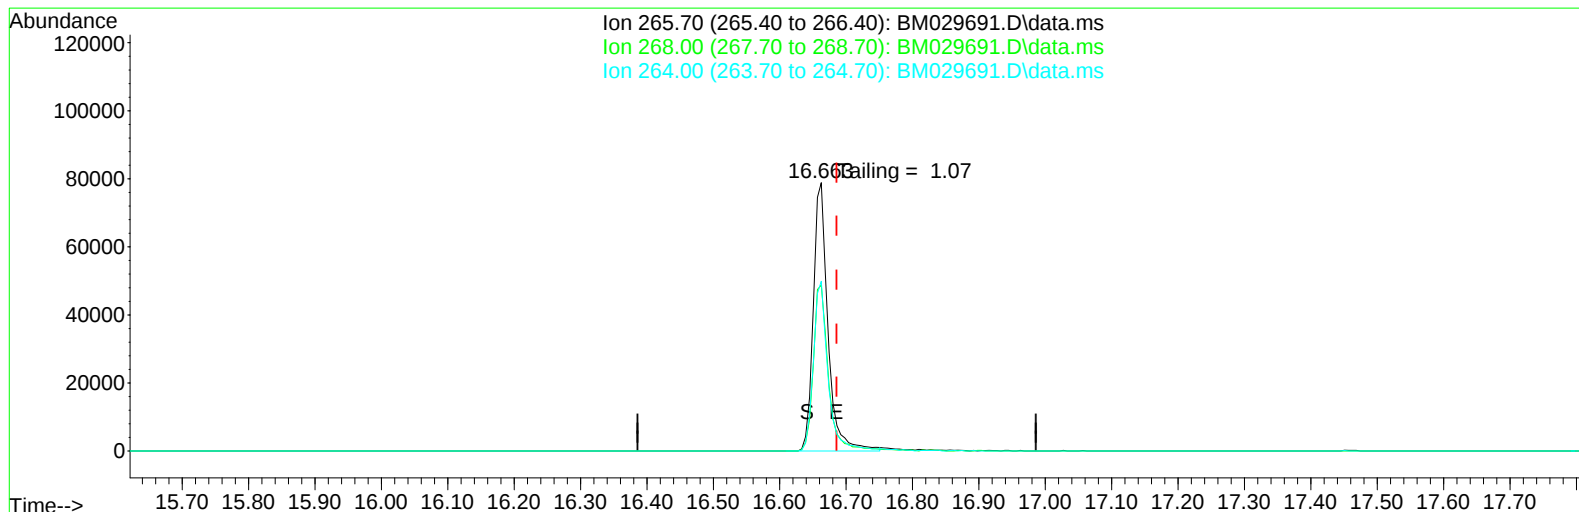

TIC: BM029691.D\data.ms

(70) Pentachlorophenol (C)

16.663min (-0.023) 0.00 ng

response 122633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	61.85
264.00	64.90	63.24
0.00	0.00	0.00