


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042921\
 Data File : BM029691.D
 Acq On : 28 Apr 2021 16:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 28 17:58:02 2021

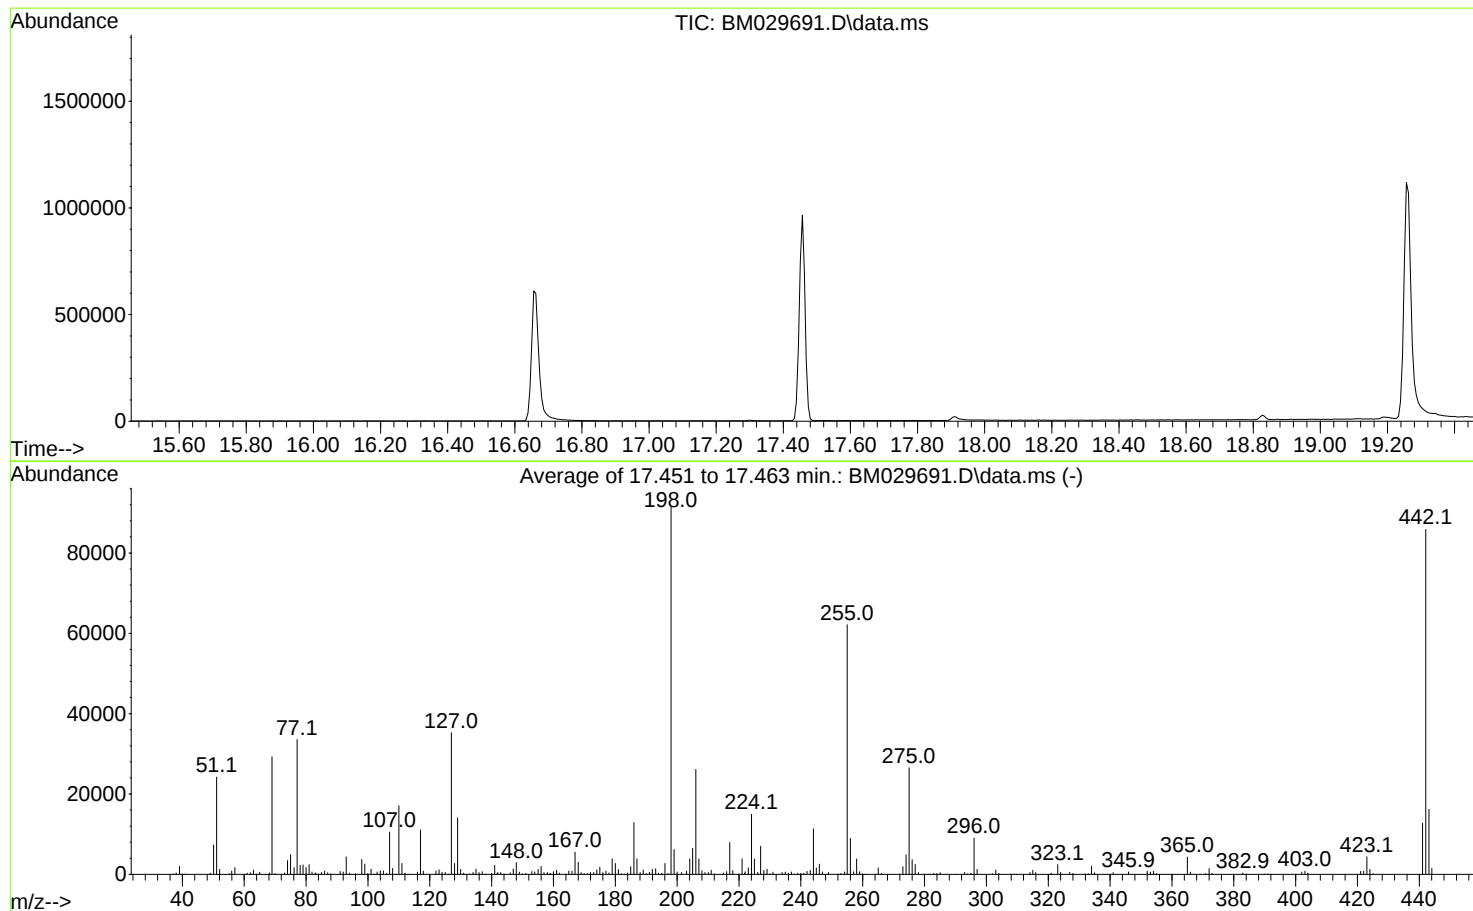

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	24165	PASS
68	69	0.00	2	1.4	418	PASS
69	198	0.00	100	32.0	29285	PASS
70	69	0.00	2	0.7	217	PASS
127	198	10	80	38.5	35235	PASS
197	198	0.00	2	0.2	215	PASS
198	198	100	100	100.0	91573	PASS
199	198	5	9	6.7	6156	PASS
275	198	10	60	29.0	26539	PASS
365	198	1	100	4.7	4319	PASS
441	198	0.01	100	13.9	12761	PASS
442	442	50	100	100.0	85896	PASS
443	442	15	24	18.8	16160	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
4/29/2021	BNA_M	<u>BM029691.D</u>
Compound Name	Response	Retention Time
DDT	396166	20.49
DDD	2713	20.05
DDE	618	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3331	399497	0.83

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042921\
Data File : BM029691.D
Acq On : 28 Apr 2021 16:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 28 16:46:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 28 09:28:15 2021
Response via : Initial Calibration

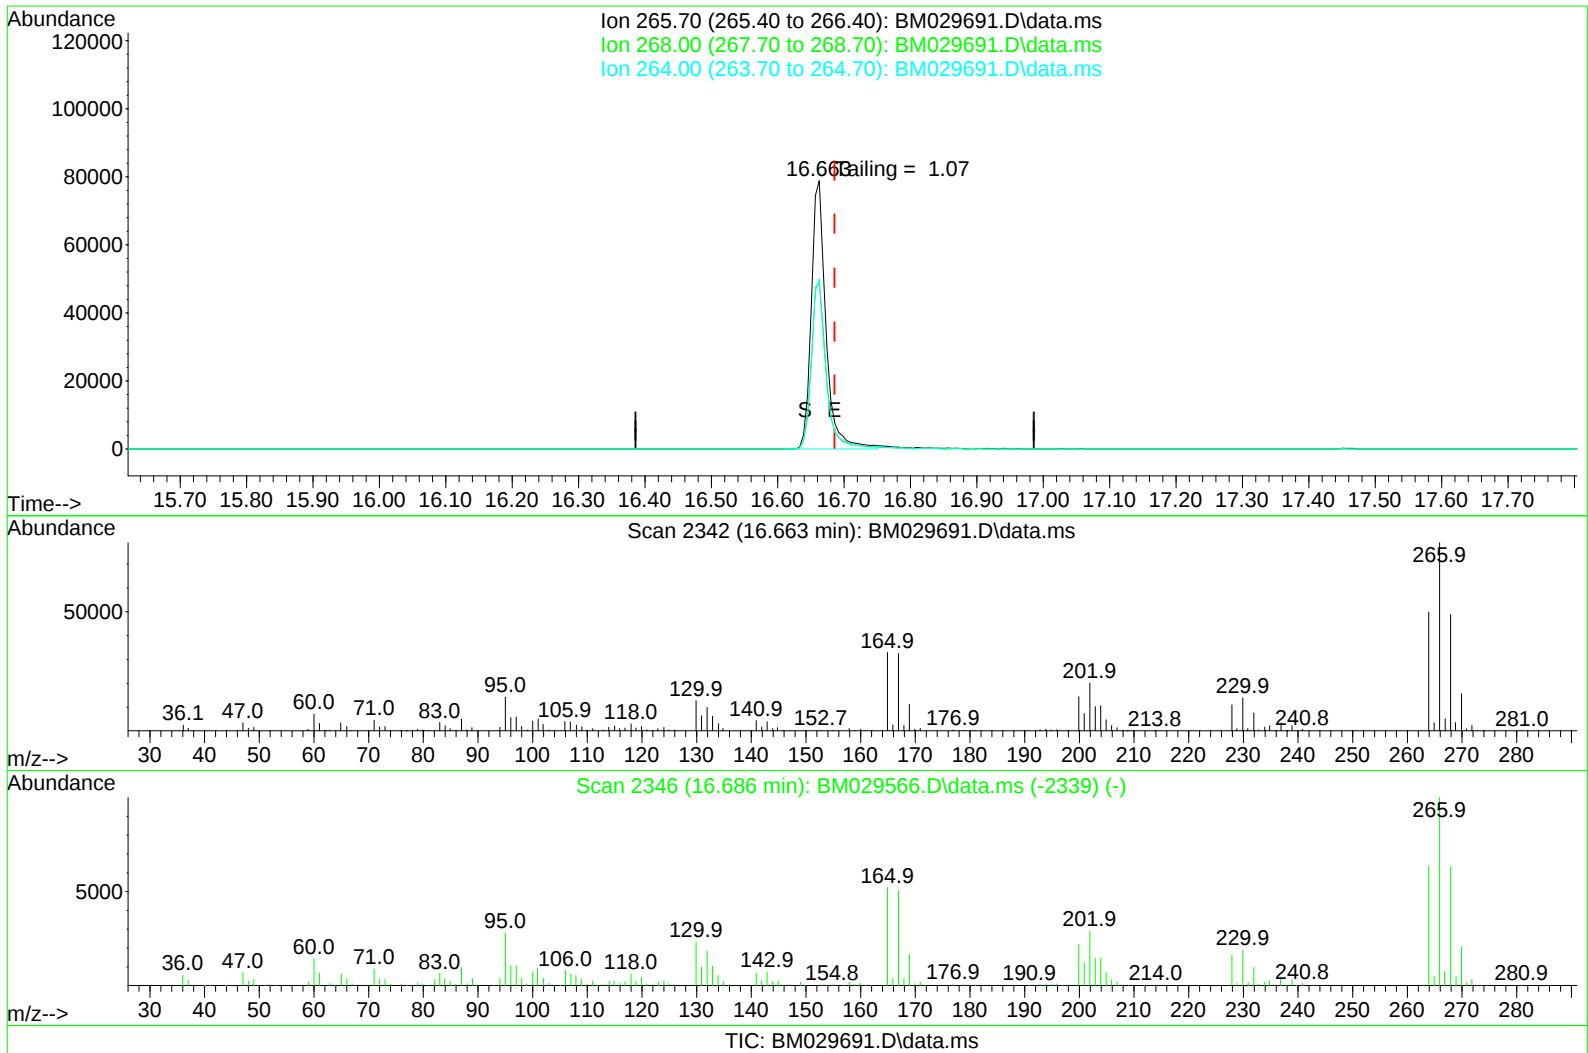

(70) Pentachlorophenol (C)

16.663min (-0.023) 0.00 ng




response 122633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	61.85
264.00	64.90	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042921\
Data File : BM029691.D
Acq On : 28 Apr 2021 16:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 28 16:46:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 28 09:28:15 2021
Response via : Initial Calibration

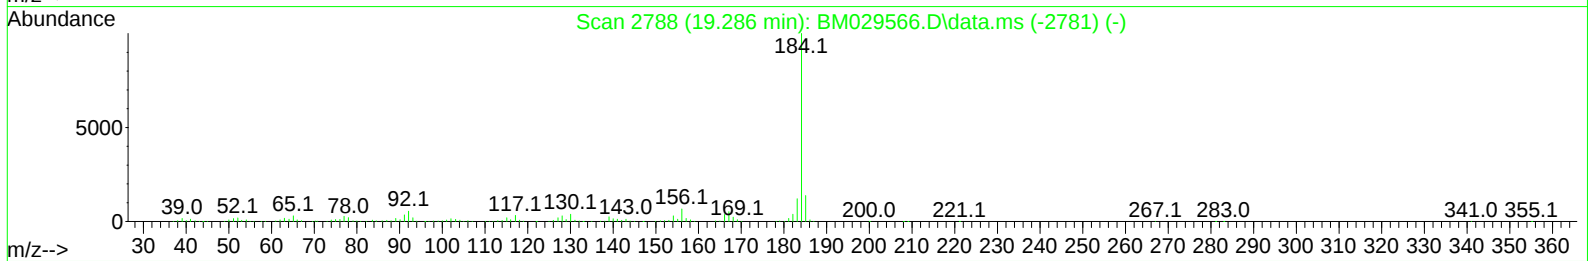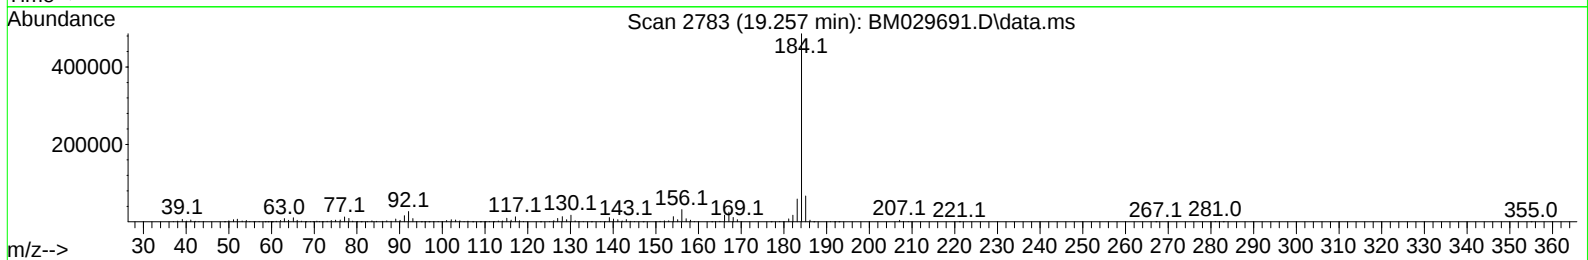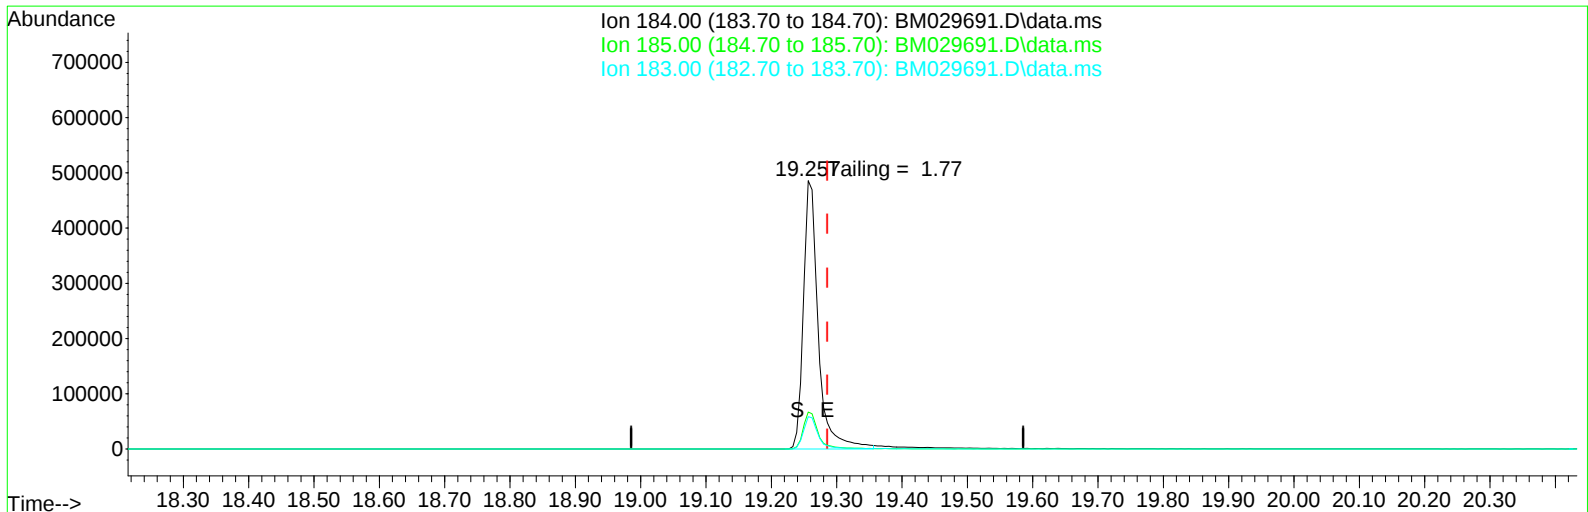

TIC: BM029691.D\data.ms

(77) Benzidine

19.257min (-0.029) 175451.73 ng

response 787521

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.77
183.00	12.30	12.09
0.00	0.00	0.00