




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
Data File : BM045632.D
Acq On : 30 Apr 2024 00:40
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Manual IntegrationsAPPROVED

Quant Time: Apr 30 01:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 30 01:16:44 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/02/2024
Supervised By :mohammad ahmed 05/02/2024

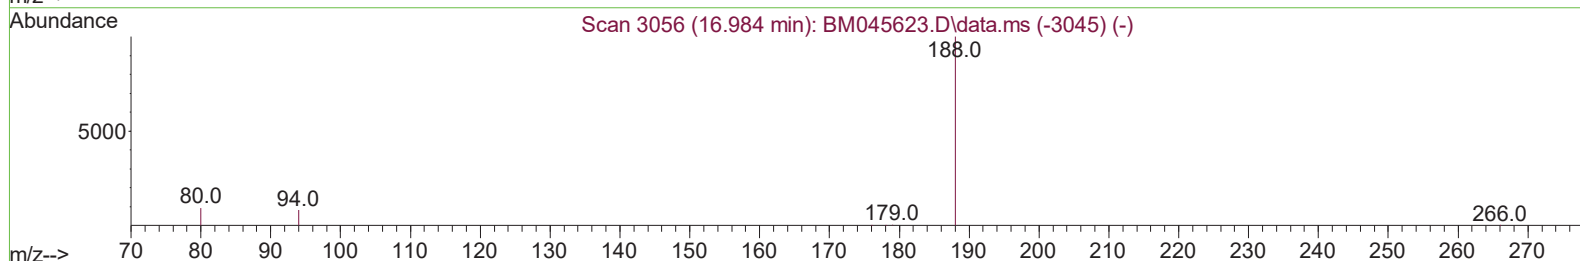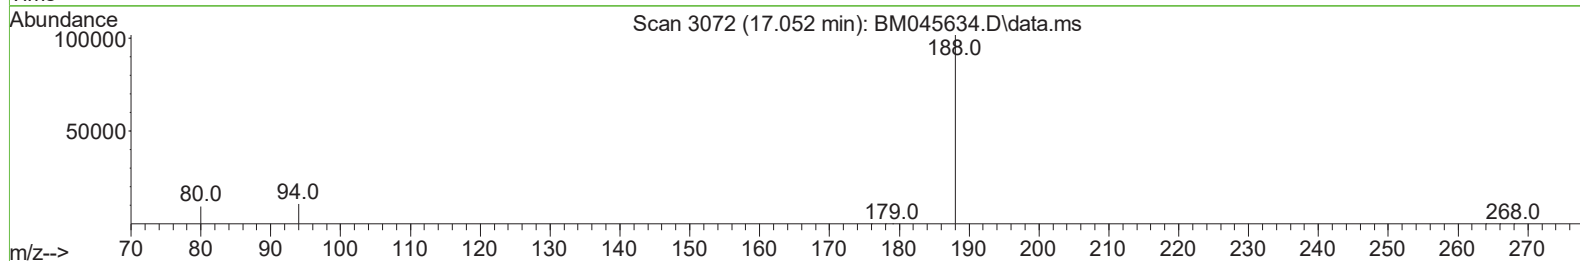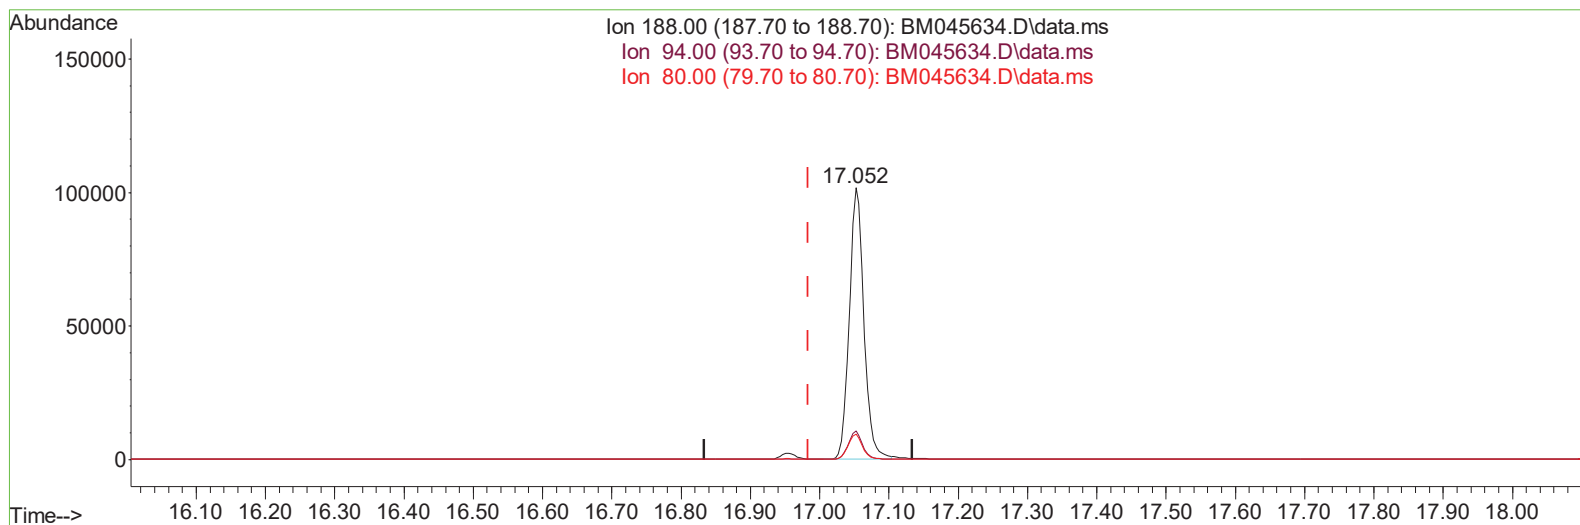

TIC: BM045634.D\data.ms

(13) Phenanthrene-d10 (I)

17.052min (+ 0.068) 0.40 ng/u1

response 149186

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	10.43#
80.00	14.80	9.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
Data File : BM045632.D
Acq On : 30 Apr 2024 00:40
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Manual IntegrationsAPPROVED

Quant Time: Apr 30 01:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 30 01:16:44 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/02/2024
Supervised By :mohammad ahmed 05/02/2024

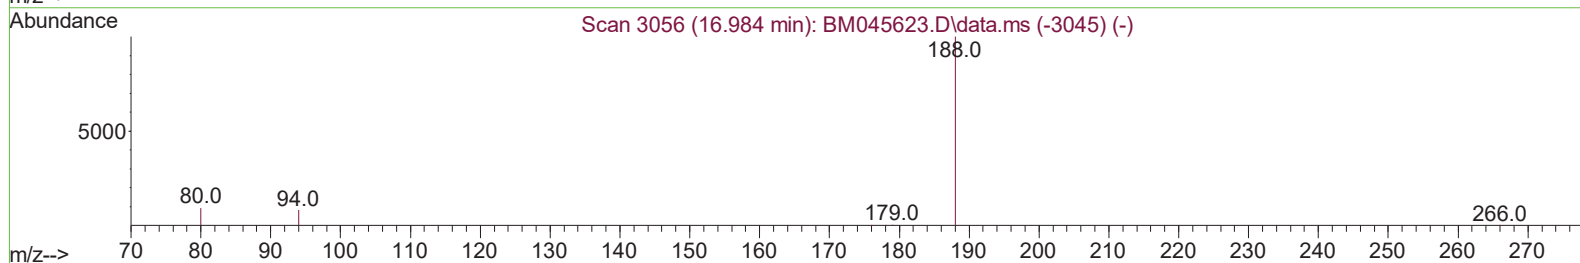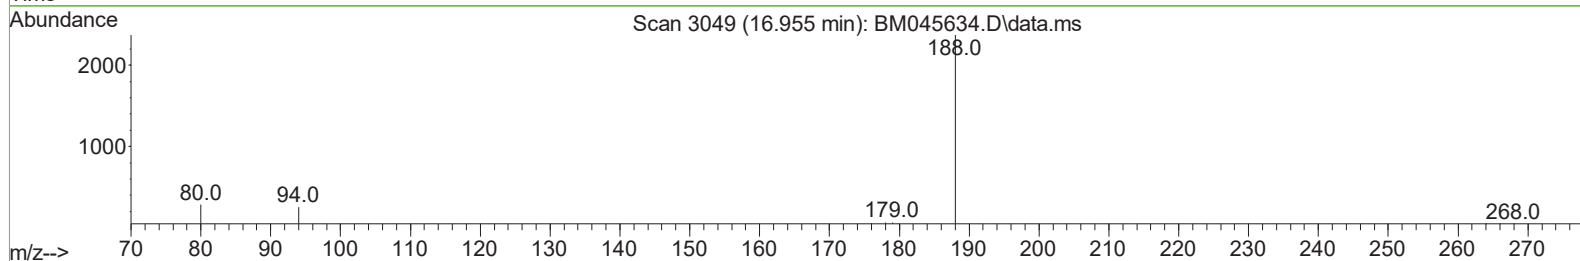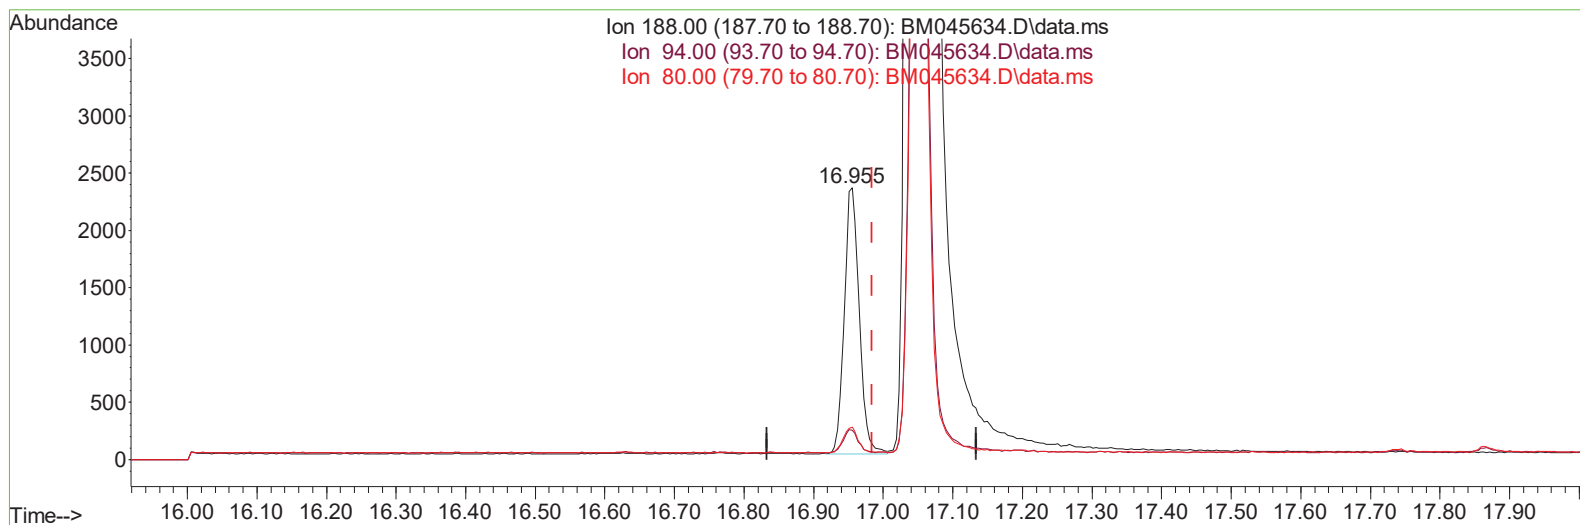

TIC: BM045634.D\data.ms

(13) Phenanthrene-d10 (I)

16.955min (-0.029) 0.40 ng/u1 m

response 3461

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	10.80#
80.00	14.80	11.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
Data File : BM045632.D
Acq On : 30 Apr 2024 00:40
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Manual IntegrationsAPPROVED

Quant Time: Apr 30 01:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 30 01:16:44 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/02/2024
Supervised By :mohammad ahmed 05/02/2024

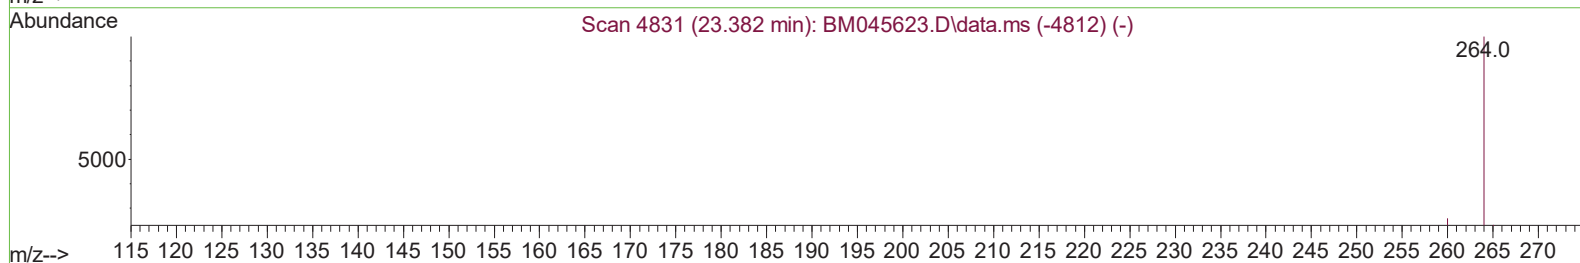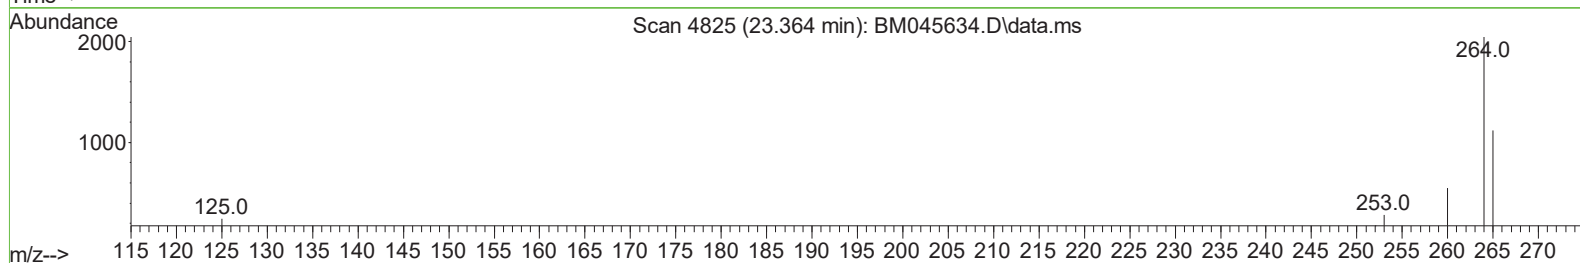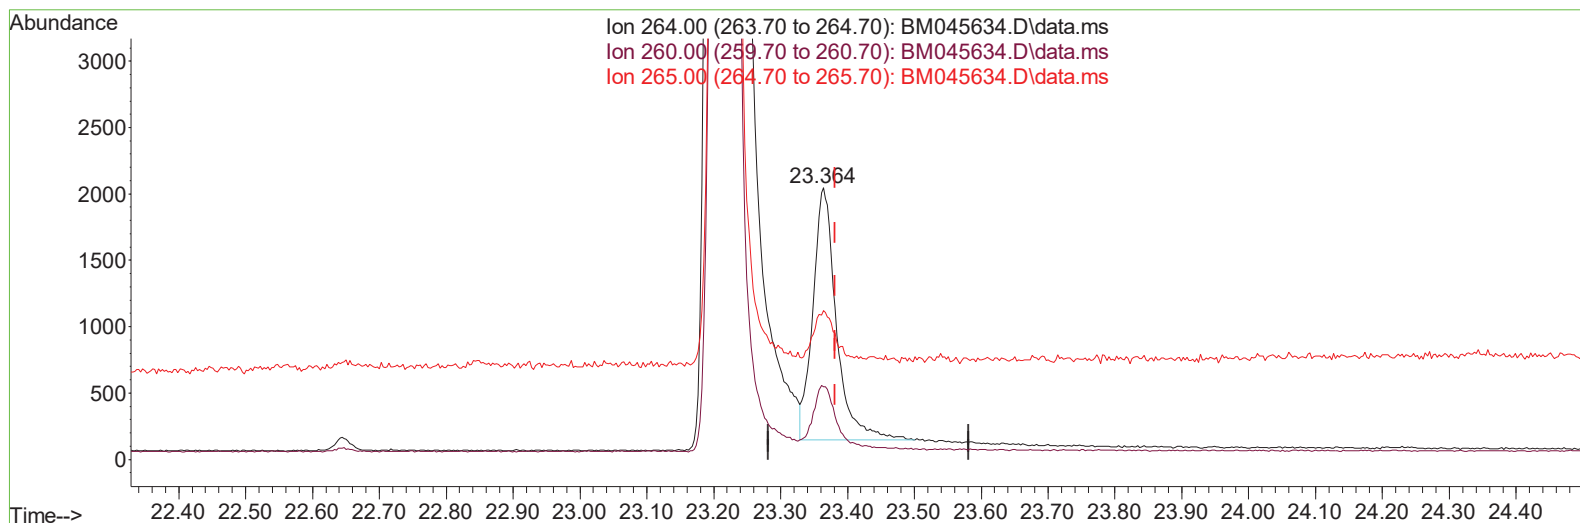

TIC: BM045634.D\data.ms

(23) Perylene-d12 (I)

23.364min (-0.019) 0.40 ng/u1

response 4620

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	30.50	26.85
265.00	86.70	54.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
Data File : BM045632.D
Acq On : 30 Apr 2024 00:40
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Manual IntegrationsAPPROVED

Quant Time: Apr 30 01:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 30 01:16:44 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/02/2024
Supervised By :mohammad ahmed 05/02/2024

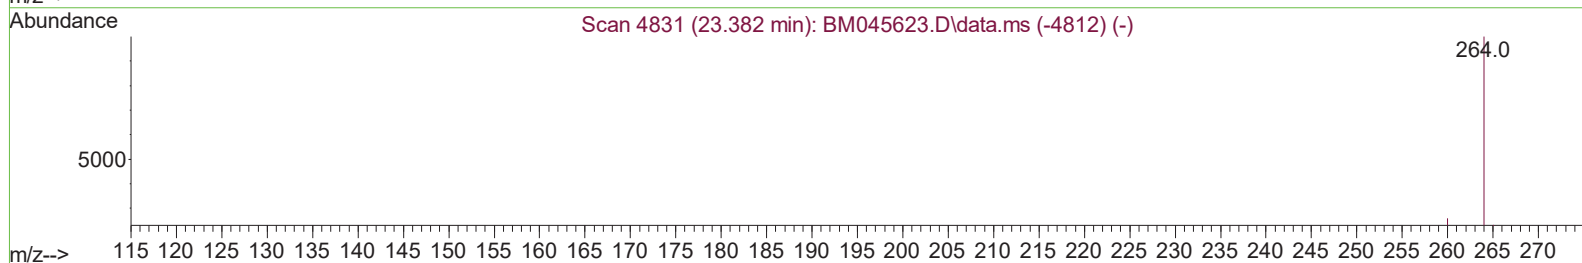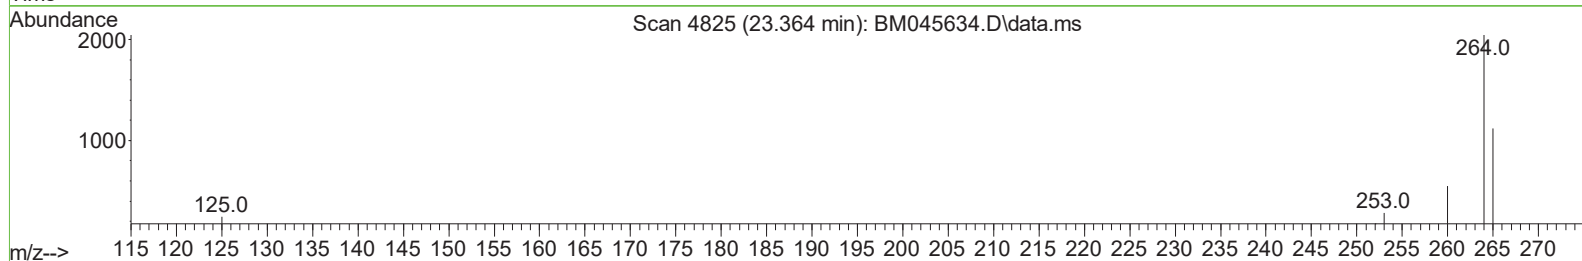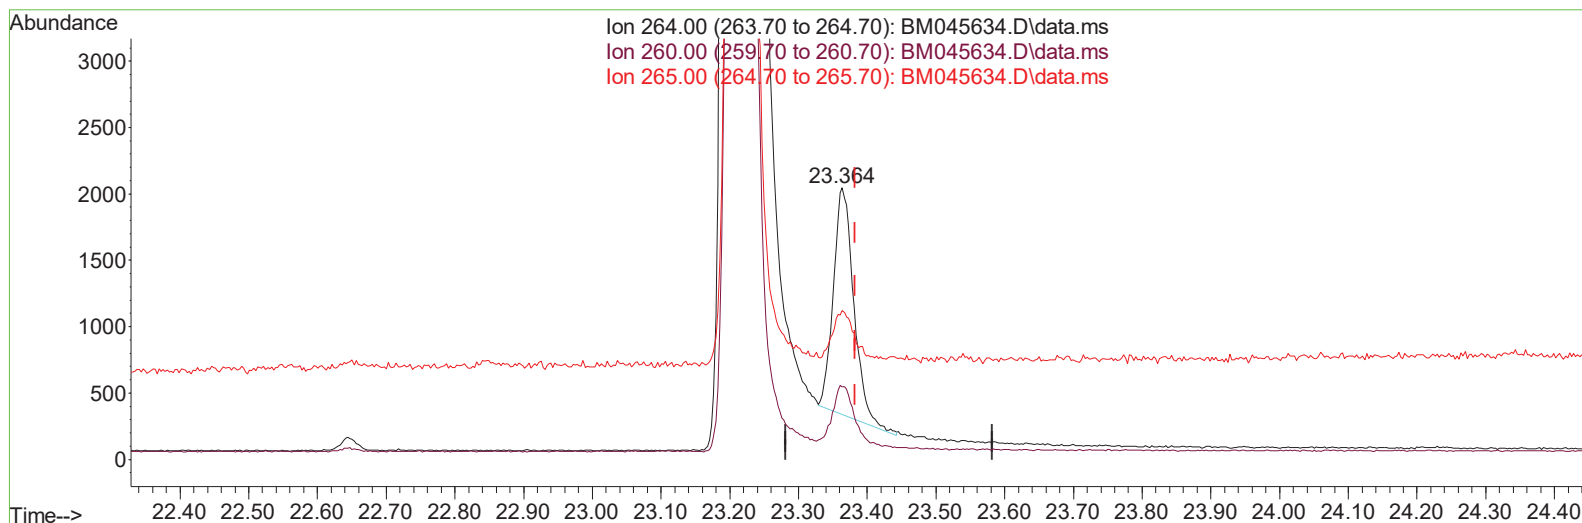

TIC: BM045634.D\data.ms

(23) Perylene-d12 (I)

23.364min (-0.019) 0.40 ng/ul m

response 3517

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	30.50	26.85
265.00	86.70	54.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
Data File : BM045632.D
Acq On : 30 Apr 2024 00:40
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Manual IntegrationsAPPROVED

Quant Time: Apr 30 01:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 30 01:16:44 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/02/2024
Supervised By :mohammad ahmed 05/02/2024

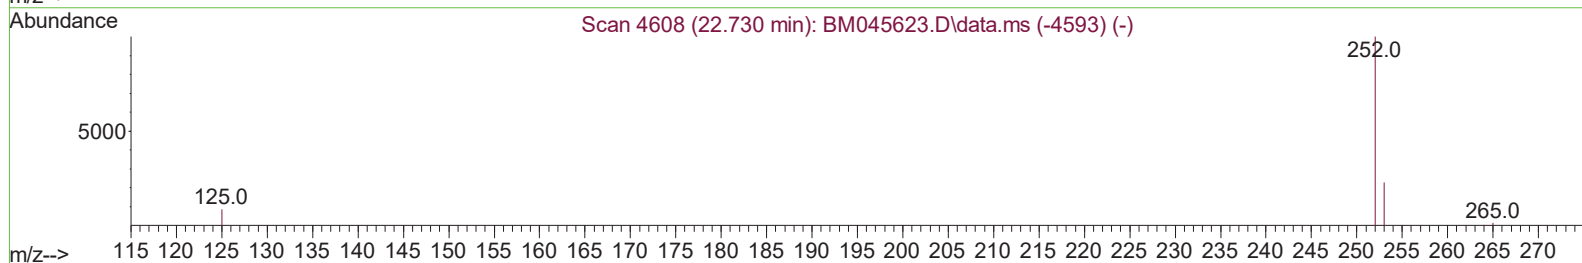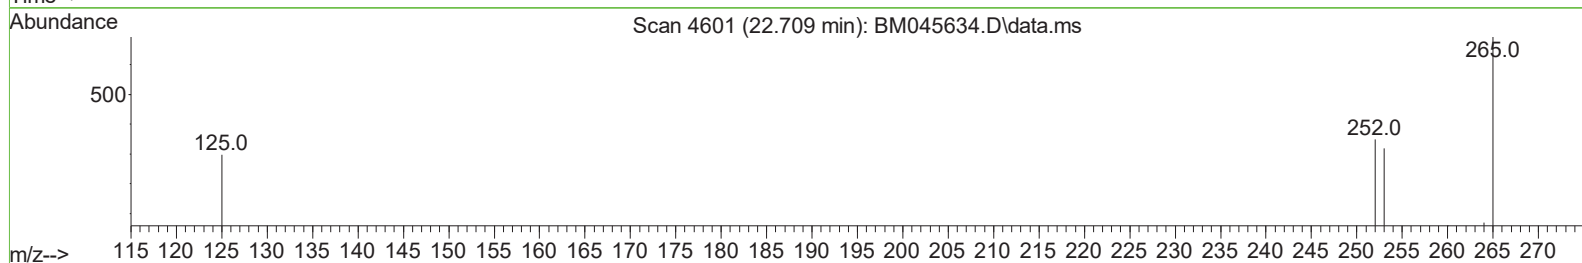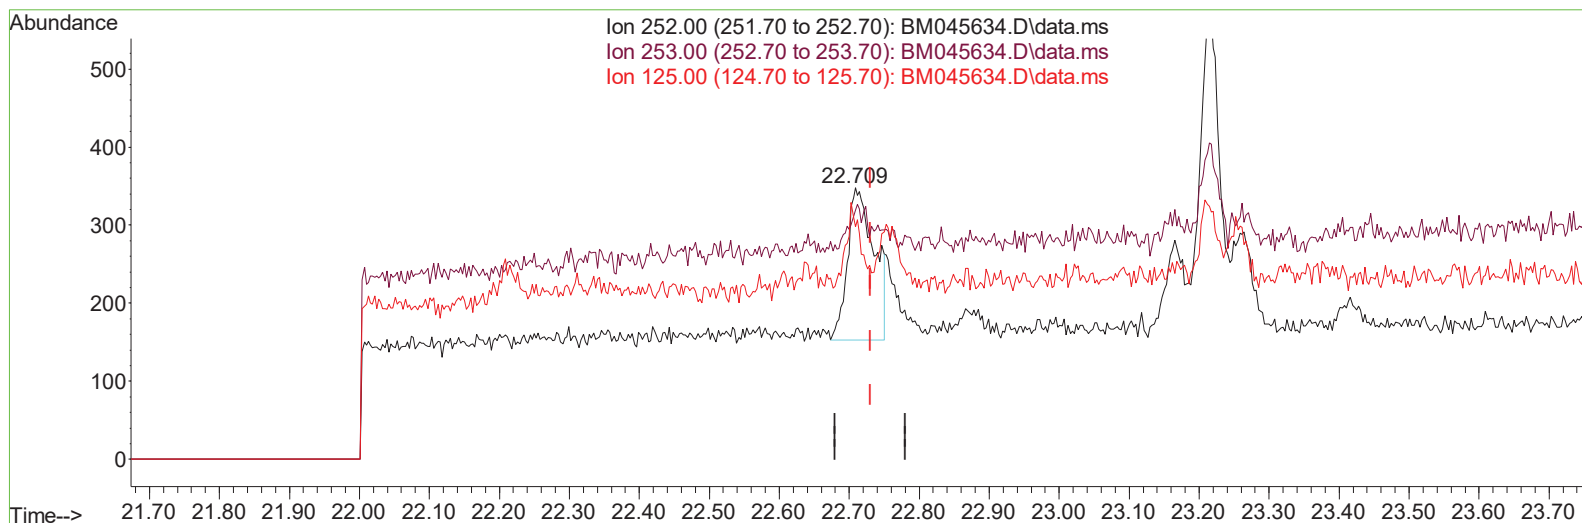

TIC: BM045634.D\data.ms

(24) Benzo(b)fluoranthene

22.709min (-0.022) 0.04 ng/u1

response 511

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.70	91.67#
125.00	18.40	85.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
Data File : BM045632.D
Acq On : 30 Apr 2024 00:40
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Manual IntegrationsAPPROVED

Quant Time: Apr 30 01:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 30 01:16:44 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 05/02/2024
Supervised By :mohammad ahmed 05/02/2024

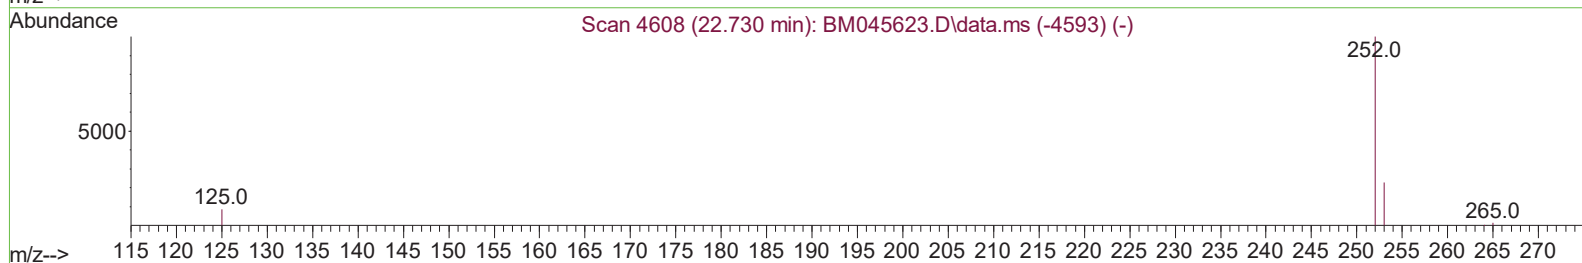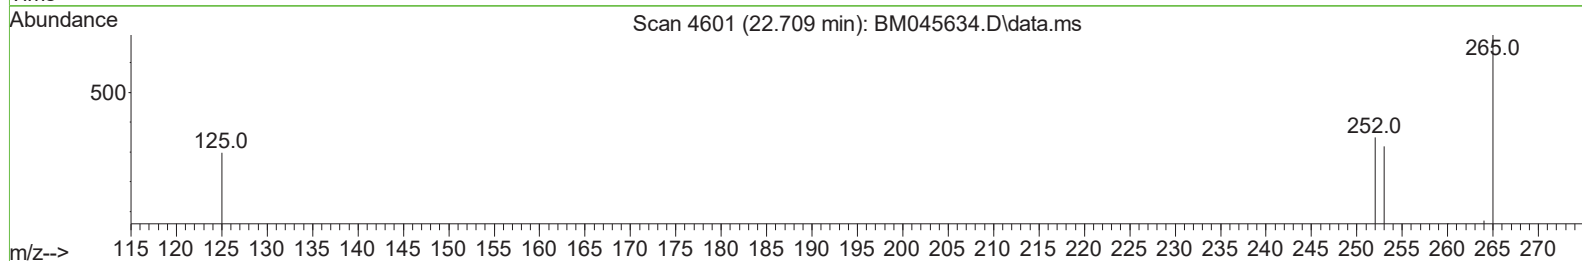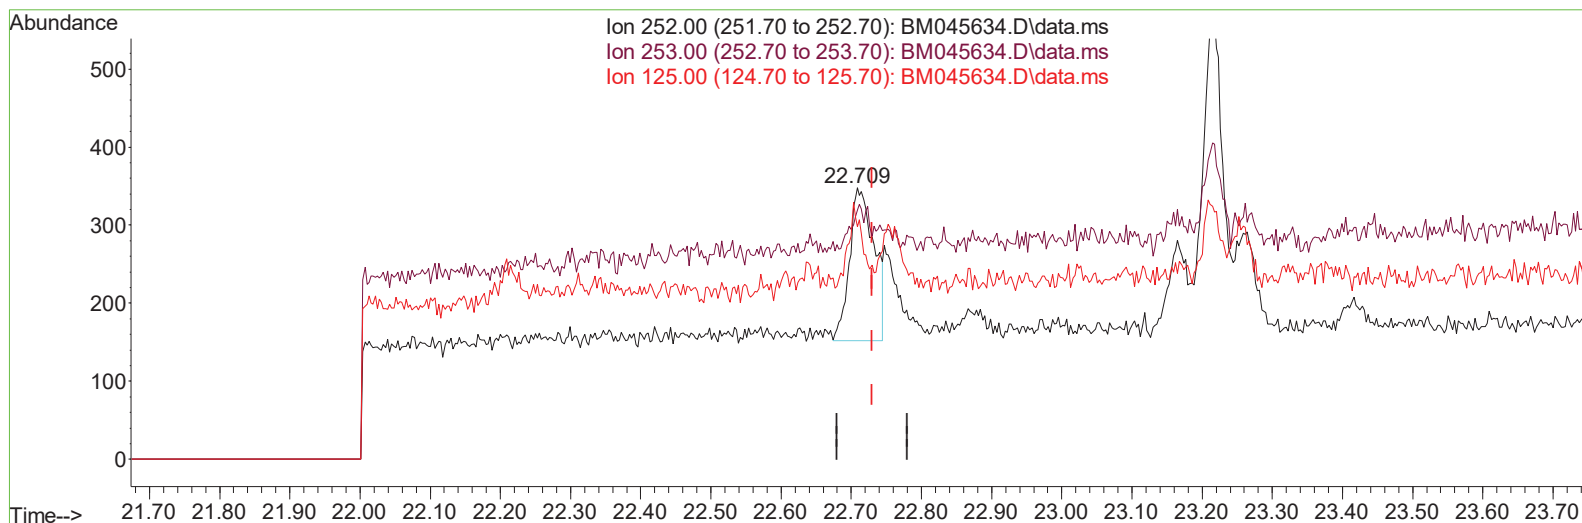

TIC: BM045634.D\data.ms

(24) Benzo(b)fluoranthene

22.709min (-0.022) 0.04 ng/u1 m

response 474

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.70	91.67#
125.00	18.40	85.63#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
 Data File : BM045632.D
 Acq On : 30 Apr 2024 00:40
 Operator : MA/JU
 Sample : P2119-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/02/2024
 Supervised By :mohammad ahmed 05/02/2024

Quant Time: Apr 30 01:19:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 30 01:16:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.538	152	1468	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.303	136	4098	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.192	164	1950	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.955	188	3461m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.189	240	2858	0.400	ng/ul	0.00
23) Perylene-d12	23.364	264	3517m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	5027	2.555	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.914	152	1125	0.208	ng/ul	-0.02
18) Fluoranthene-d10	19.002	212	1654	0.184	ng/ul	-0.02
Target Compounds						
					Qvalue	
5) Naphthalene	10.352	128	276	0.025	ng/ul#	59
7) 2-Methylnaphthalene	11.991	142	145	0.023	ng/ul	92
19) Fluoranthene	19.030	202	441	0.033	ng/ul#	59
20) Pyrene	19.392	202	360	0.027	ng/ul#	46
21) Benzo(a)anthracene	21.178	228	245	0.027	ng/ul#	57
24) Benzo(b)fluoranthene	22.709	252	474m	0.040	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042924\
Data File : BM045632.D
Acq On : 30 Apr 2024 00:40
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/02/2024
Supervised By :mohammad ahmed 05/02/2024

Quant Time: Apr 30 01:19:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 30 01:16:44 2024
Response via : Initial Calibration

