

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
 Data File : BM005147.D
 Acq On : 29 Apr 2016 17:55
 Operator : UM/SJ
 Sample : H2778-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B63

Quant Time: Apr 30 03:09:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	31331	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	156178	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	105633	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	250052	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	271314	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	217532	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	923	1.50	ng/uL	0.00
5) Phenol-d5	6.96	99	18097	6.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	55862	37.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	58031	28.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	37764	17.19	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	36494	33.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	41626	34.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	70704	30.84	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.83	166	283037	33.93	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	335972	33.82	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	4523	3.10	ng/ul	0.00
57) Fluorene-d10	15.42	176	246029	33.56	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	34427	24.21	ng/ul	0.00
70) Anthracene-d10	17.27	188	389756	34.76	ng/ul	0.00
76) Pyrene-d10	19.57	212	435114	35.23	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	345988	35.50	ng/ul	0.00


Target Compounds						Qvalue
45) 2,6-Dinitrotoluene	13.84	165	1842	1.14	ng/ul#	37
81) Bis(2-ethylhexyl)phthalate	21.27	149	24899	2.94	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005147.D
Acq On : 29 Apr 2016 17:55
Operator : UM/SJ
Sample : H2778-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B63

Quant Time: Apr 30 03:09:33 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 30 03:07:27 2016
Response via : Initial Calibration




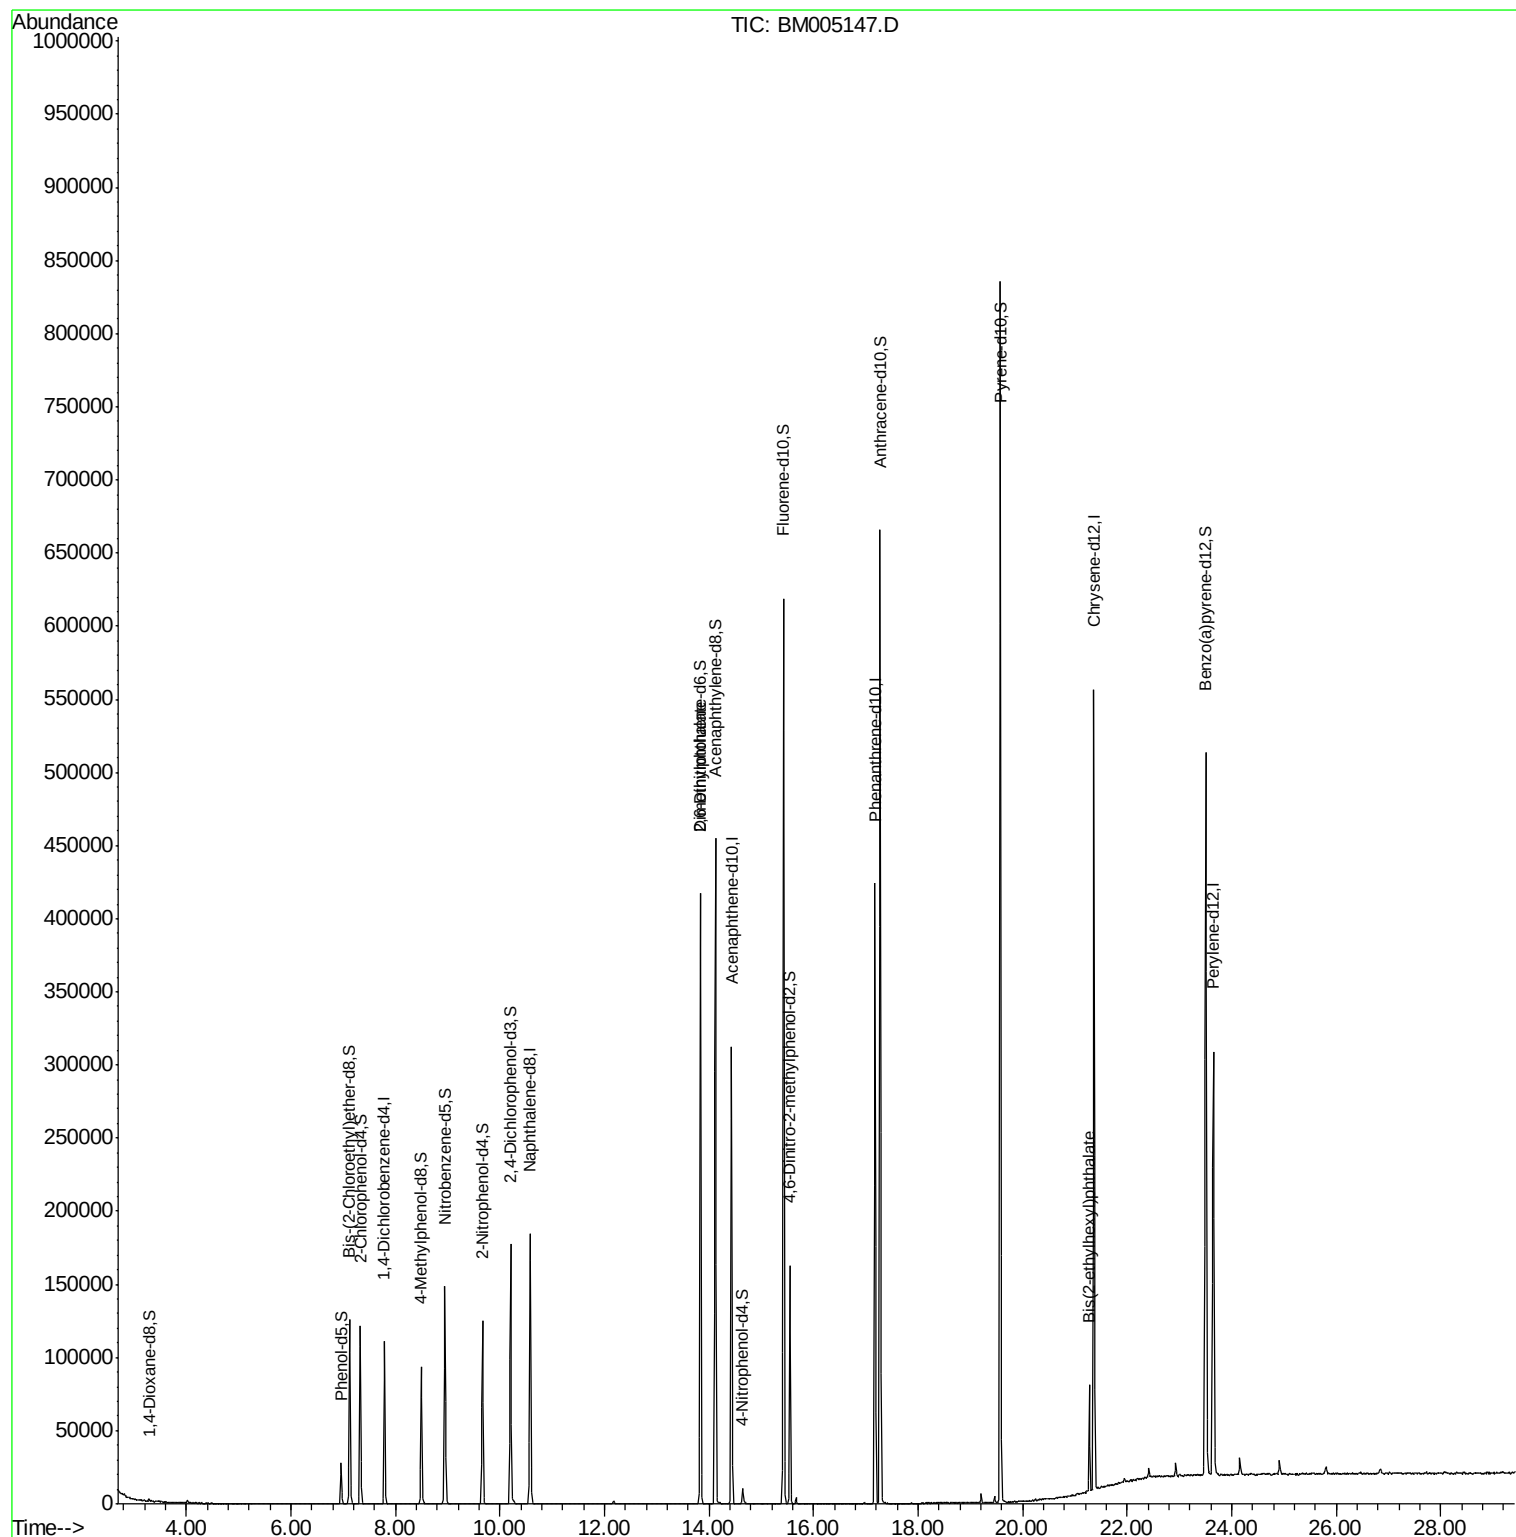


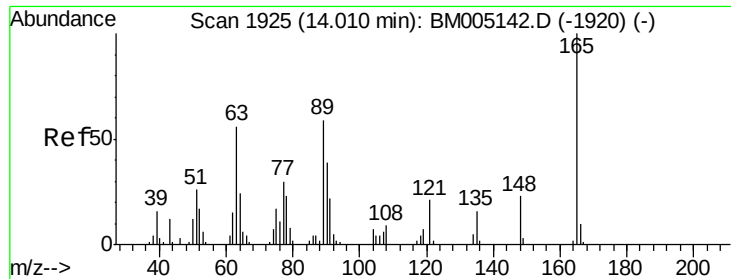

#45
 2,6-Dinitrotoluene
 Concen: 1.14 ng/ul
 RT: 13.84 min Scan# 1896
 Delta R.T. -0.17 min
 Lab File: BM005147.D
 Acq: 29 Apr 2016 17:55

Instrument :
 BNA_M
 ClientSampleId :
 C0B63

Tgt Ion:165 Resp: 1842
 Ion Ratio Lower Upper
 165 100
 89 0.0 43.1 64.7#
 121 34.0 16.0 24.0#

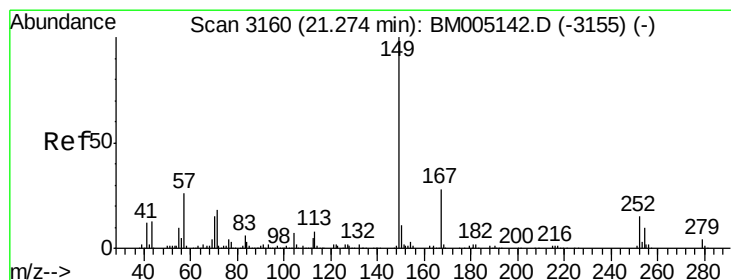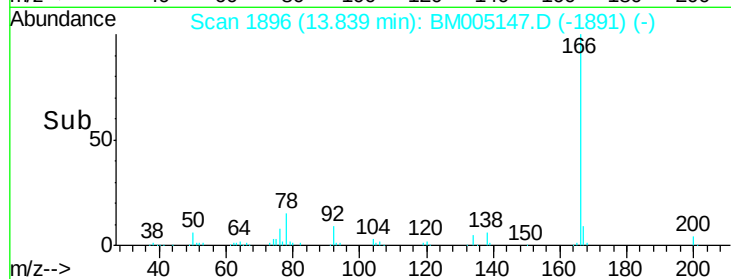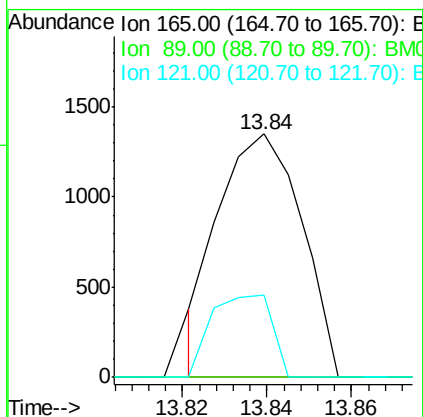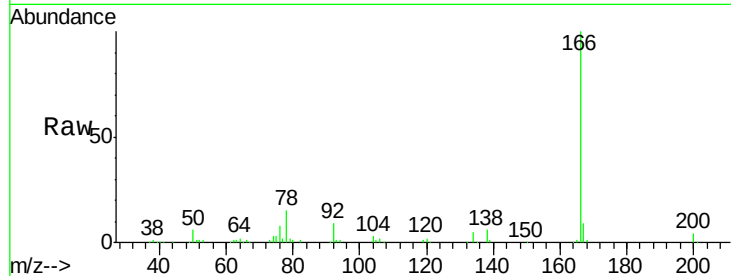

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 2.94 ng/ul
 RT: 21.27 min Scan# 3160
 Delta R.T. 0.00 min
 Lab File: BM005147.D
 Acq: 29 Apr 2016 17:55

Tgt Ion:149 Resp: 24899
 Ion Ratio Lower Upper
 149 100
 167 28.6 22.7 34.1
 279 4.3 3.4 5.0

