

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
 Data File : BM005174.D
 Acq On : 30 Apr 2016 15:22
 Operator : UM/SJ
 Sample : H2782-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC3

Quant Time: May 01 04:15:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 01 04:14:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	38122	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	180298	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	113683	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	248532	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	219414	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	195958	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	821	1.09	ng/uL	0.00
5) Phenol-d5	6.96	99	18248	5.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	57983	32.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	59572	23.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	37589	14.06	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	39556	31.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	44631	32.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	72851	27.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	5777	1.86	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	281355	31.34	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	338733	31.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	4295	2.74	ng/ul	0.00
57) Fluorene-d10	15.42	176	243405	30.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	32614	23.07	ng/ul	0.00
70) Anthracene-d10	17.27	188	363723	32.64	ng/ul	0.00
76) Pyrene-d10	19.57	212	362031	36.24	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	286751	32.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.84	165	1755	1.01	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005174.D
Acq On : 30 Apr 2016 15:22
Operator : UM/SJ
Sample : H2782-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC3

Quant Time: May 01 04:15:40 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 01 04:14:40 2016
Response via : Initial Calibration

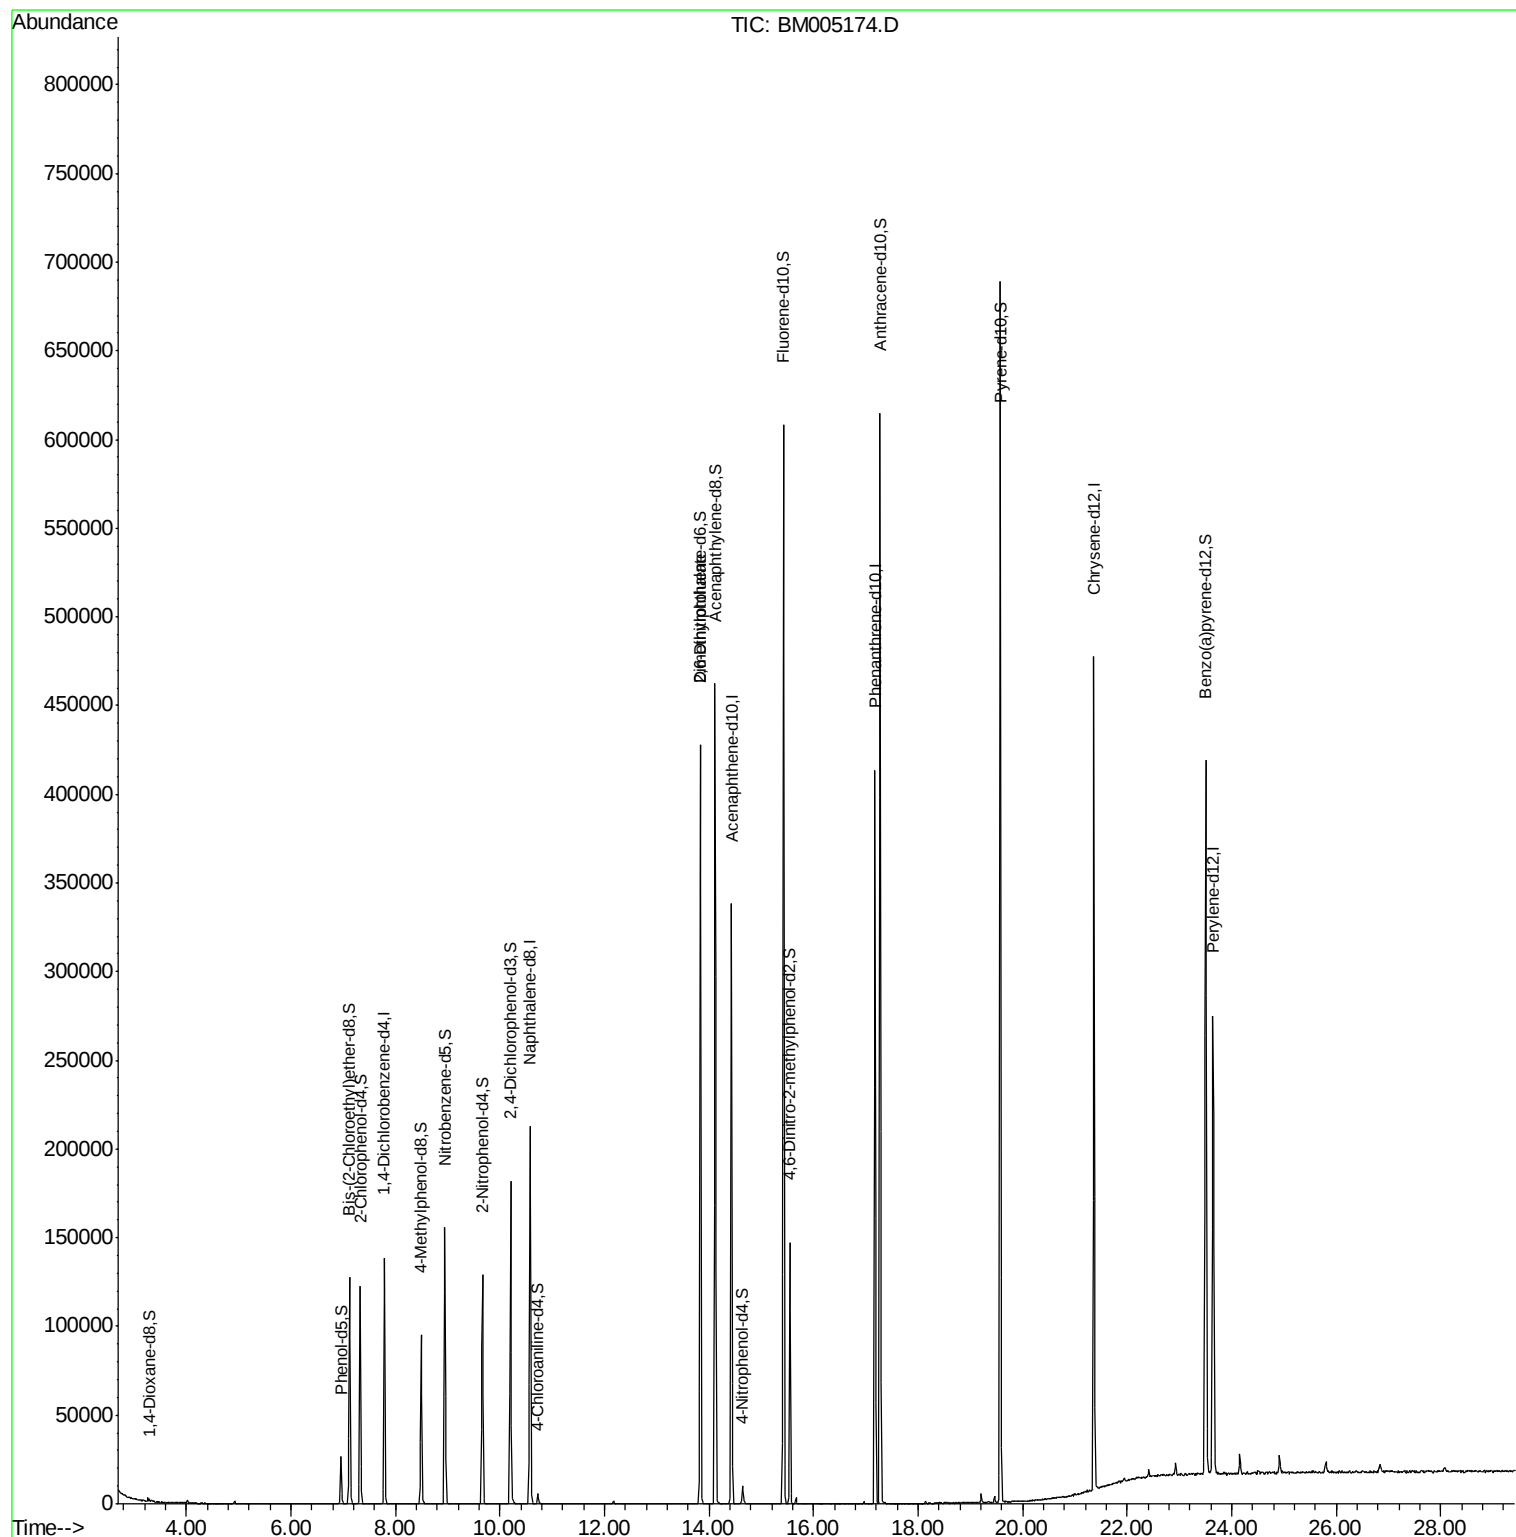

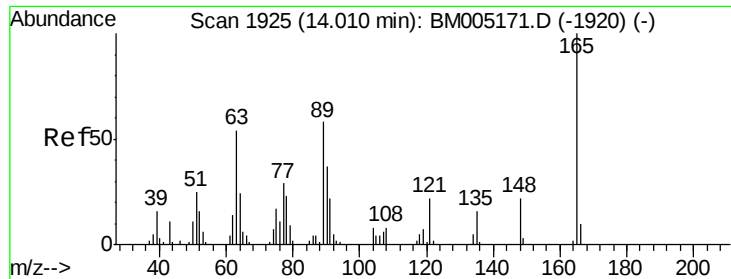

#45
 2,6-Dinitrotoluene
 Concen: 1.01 ng/ul
 RT: 13.84 min Scan# 1896
 Delta R.T. -0.17 min
 Lab File: BM005174.D
 Acq: 30 Apr 2016 15:22

Instrument :
 BNA_M
 ClientSampleId :
 C0AC3

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	43.1	64.7#
121	26.1	16.0	24.0#

