

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
 Data File : BM005180.D
 Acq On : 30 Apr 2016 18:59
 Operator : UM/SJ
 Sample : H2782-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD6

Quant Time: May 01 04:16:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 01 04:14:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	37519	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	181646	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	118423	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	262751	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	235204	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	208221	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	2721	3.69	ng/uL	-0.03
5) Phenol-d5	6.96	99	18060	5.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	59092	33.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	61168	24.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	37980	14.43	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	39817	31.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	44406	31.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	74481	27.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	5029	1.61	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	293428	31.37	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	345742	31.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	4140	2.53	ng/ul	0.00
57) Fluorene-d10	15.42	176	253211	30.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	35613	23.83	ng/ul	0.00
70) Anthracene-d10	17.27	188	383936	32.59	ng/ul	0.00
76) Pyrene-d10	19.57	212	385975	36.05	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	304467	32.64	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.83	165	1842	1.02 ng/ul#	37




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005180.D
Acq On : 30 Apr 2016 18:59
Operator : UM/SJ
Sample : H2782-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD6

Quant Time: May 01 04:16:19 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 01 04:14:40 2016
Response via : Initial Calibration

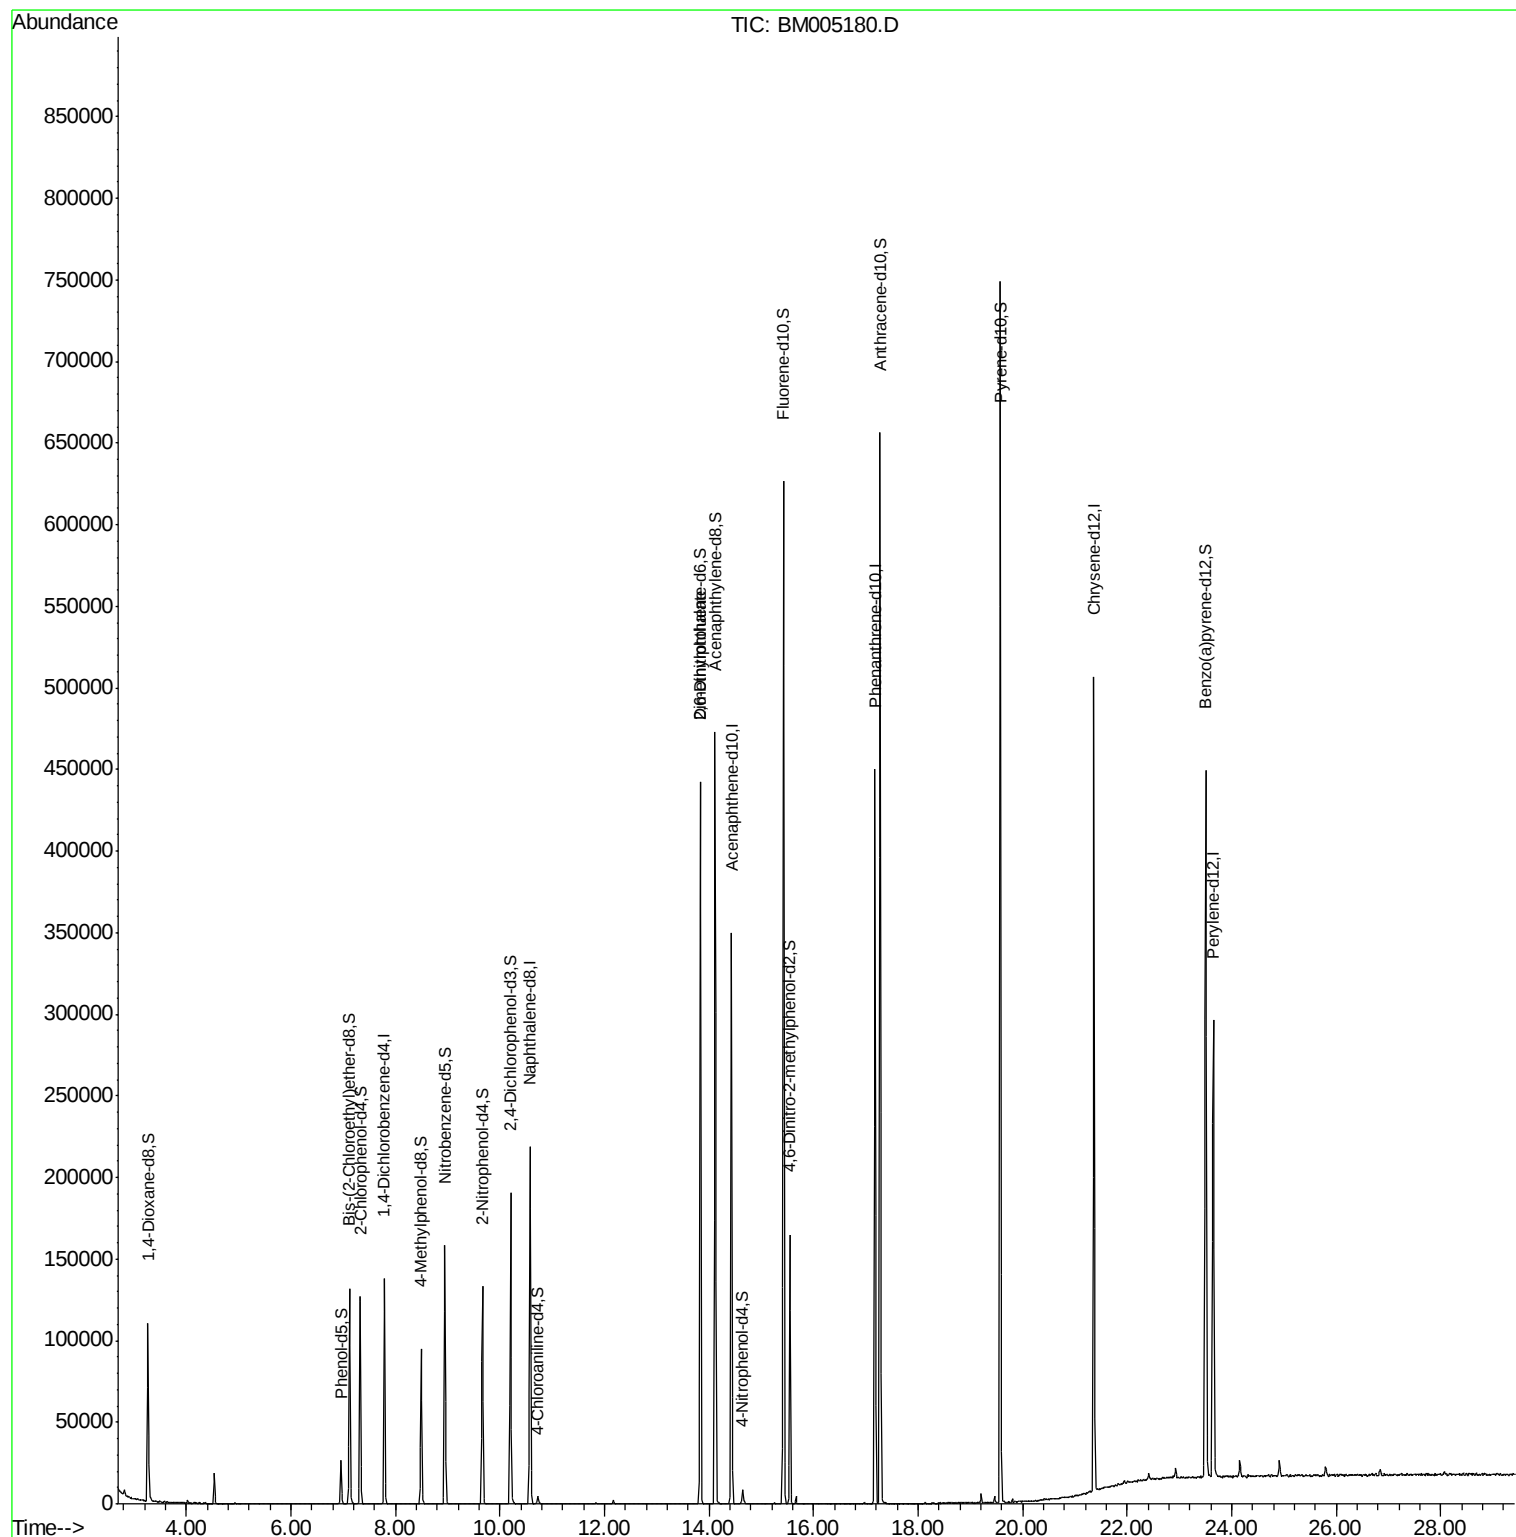

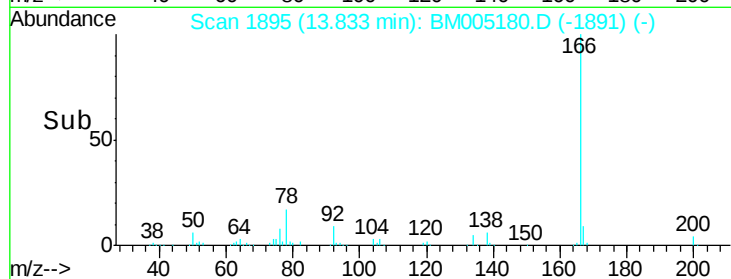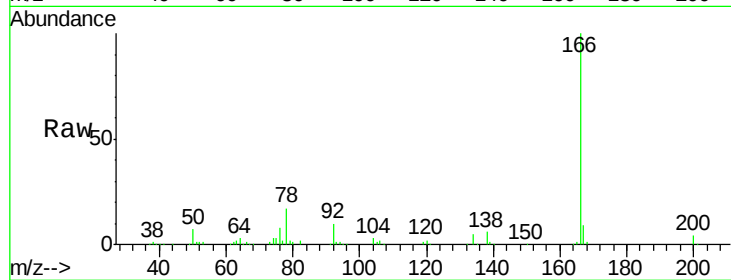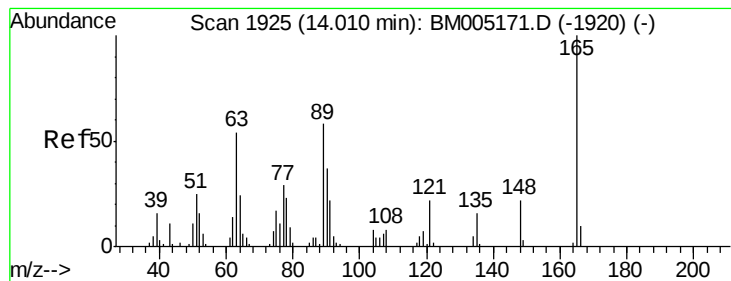

#45

2,6-Dinitrotoluene

Concen: 1.02 ng/ul

RT: 13.83 min Scan# 1895

Delta R.T. -0.18 min

Lab File: BM005180.D

Acq: 30 Apr 2016 18:59

Instrument :

BNA_M

ClientSampleId :

C0AD6

Tgt Ion:165 Resp: 1842

Ion Ratio Lower Upper

165 100

89 0.0 43.1 64.7#

121 34.3 16.0 24.0#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

