

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
 Data File : BM005183.D
 Acq On : 30 Apr 2016 20:48
 Operator : UM/SJ
 Sample : H2782-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD9

Quant Time: May 01 04:16:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 01 04:14:40 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	40511	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	192841	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	121843	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	274058	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	241976	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	214267	20.00	ng/ul	0.00




System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	978	1.23	ng/uL	0.00
5) Phenol-d5	6.96	99	18391	5.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	57402	30.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	59871	22.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	38728	13.63	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	38864	29.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	44053	29.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	72454	25.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	4577	1.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	286929	29.82	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	340490	29.71	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	4284	2.55	ng/ul	0.00
57) Fluorene-d1						

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005183.D
Acq On : 30 Apr 2016 20:48
Operator : UM/SJ
Sample : H2782-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD9

Quant Time: May 01 04:16:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 01 04:14:40 2016
Response via : Initial Calibration

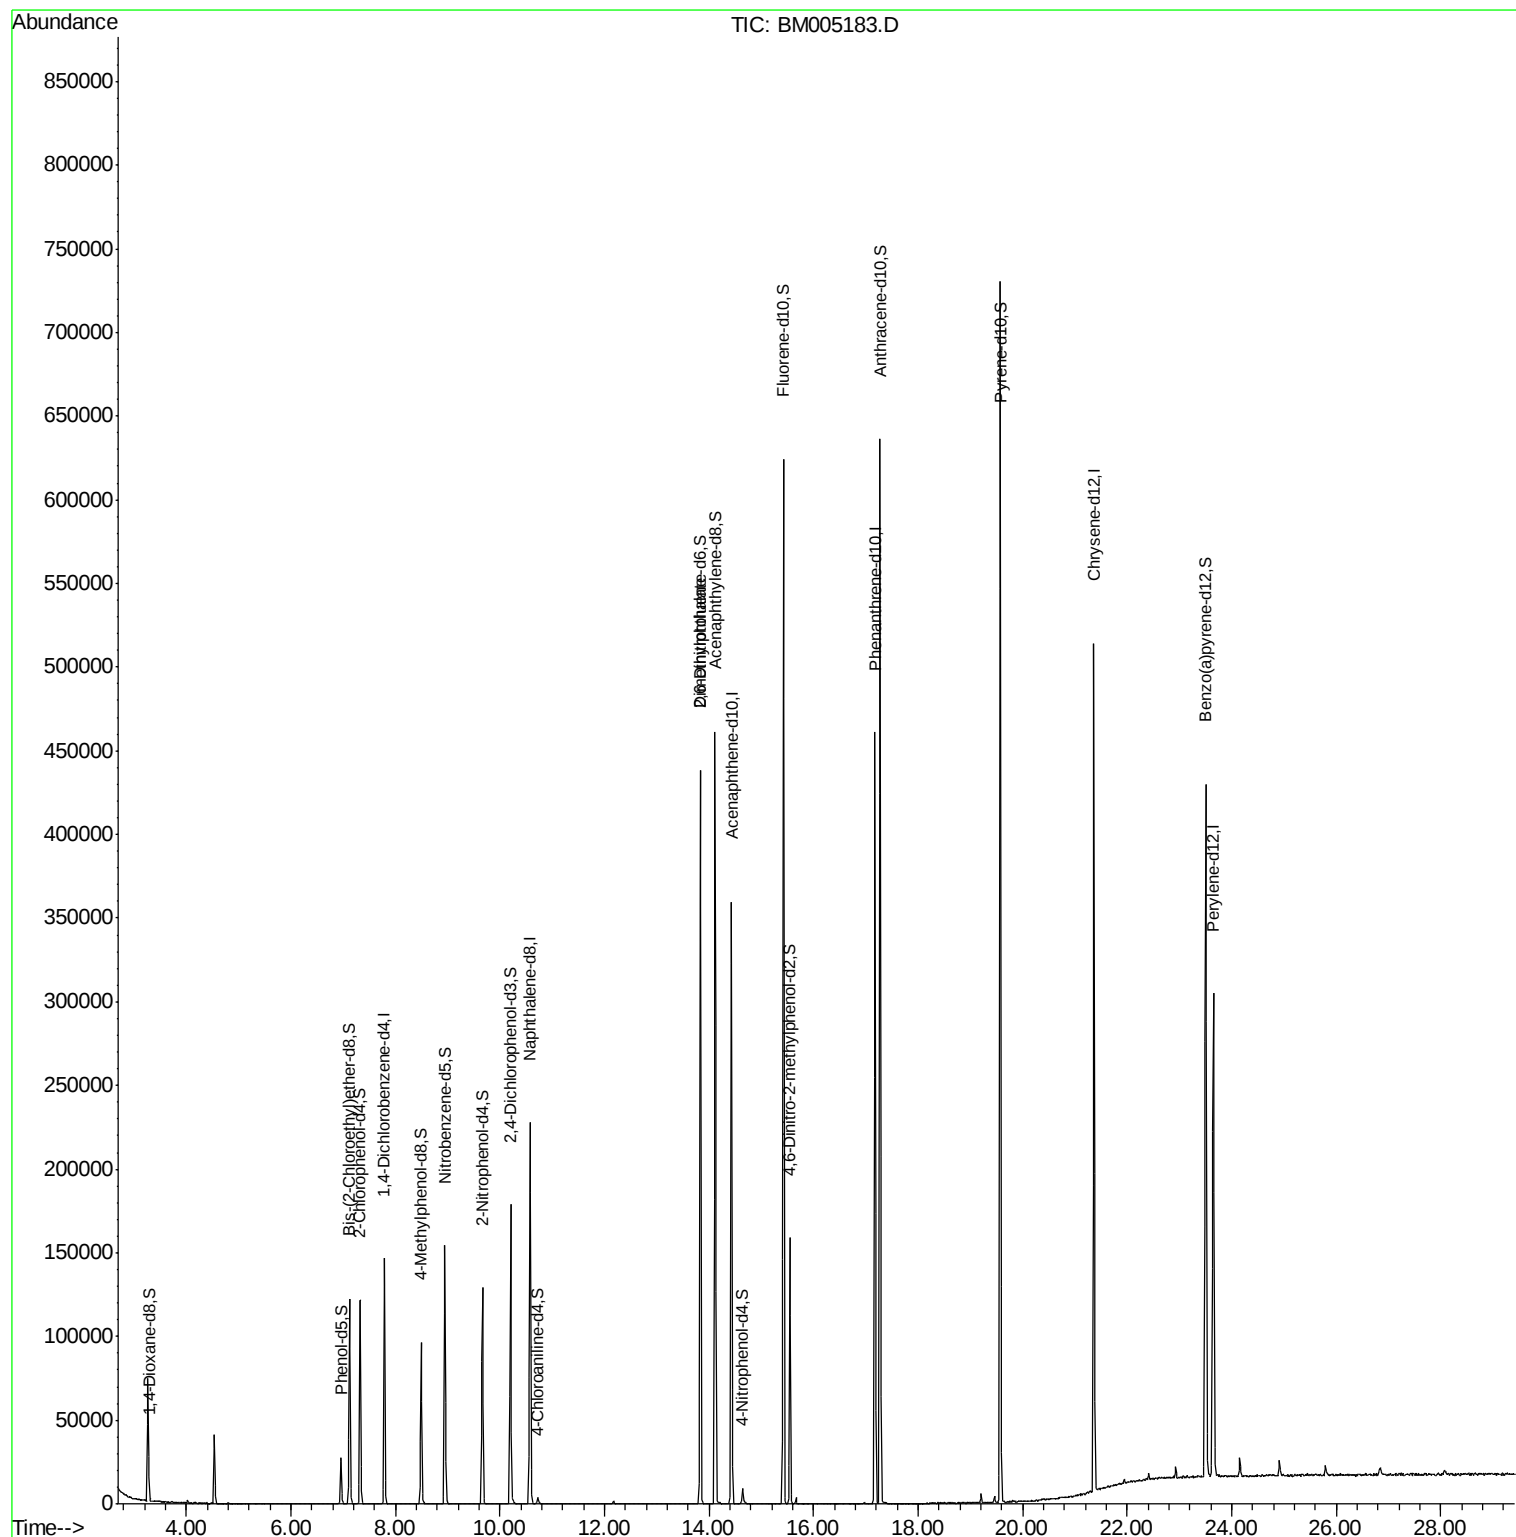

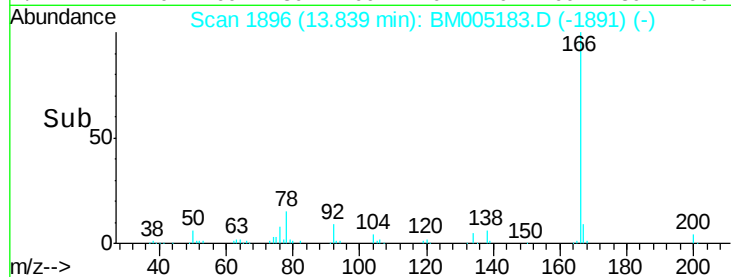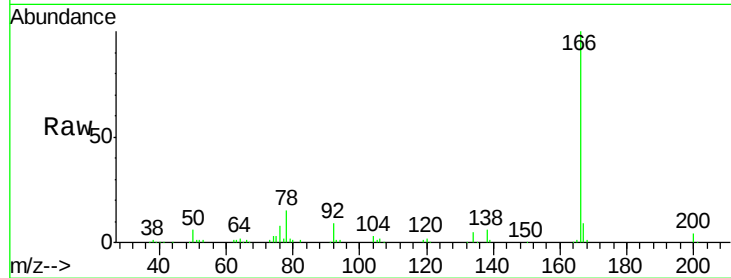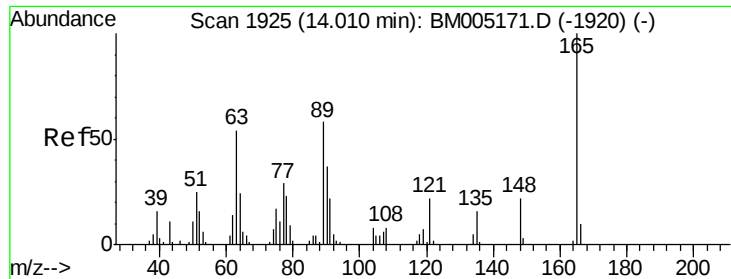

#45

2,6-Dinitrotoluene

Concen: 1.00 ng/ul

RT: 13.84 min Scan# 1896

Delta R.T. -0.17 min

Lab File: BM005183.D

Acq: 30 Apr 2016 20:48

Instrument :

BNA_M

ClientSampleId :

C0AD9

Tgt Ion:165 Resp: 1864

Ion Ratio Lower Upper

165 100

89 0.0 43.1 64.7#

121 24.6 16.0 24.0#

