

Quantitation Report (LSC Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM043016\
 Data File : BM005158.D
 Acq On : 30 Apr 2016 01:10
 Operator : UM/SJ
 Sample : H2729-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B8

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:40 AM

Quant Time: Apr 30 04:41:34 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

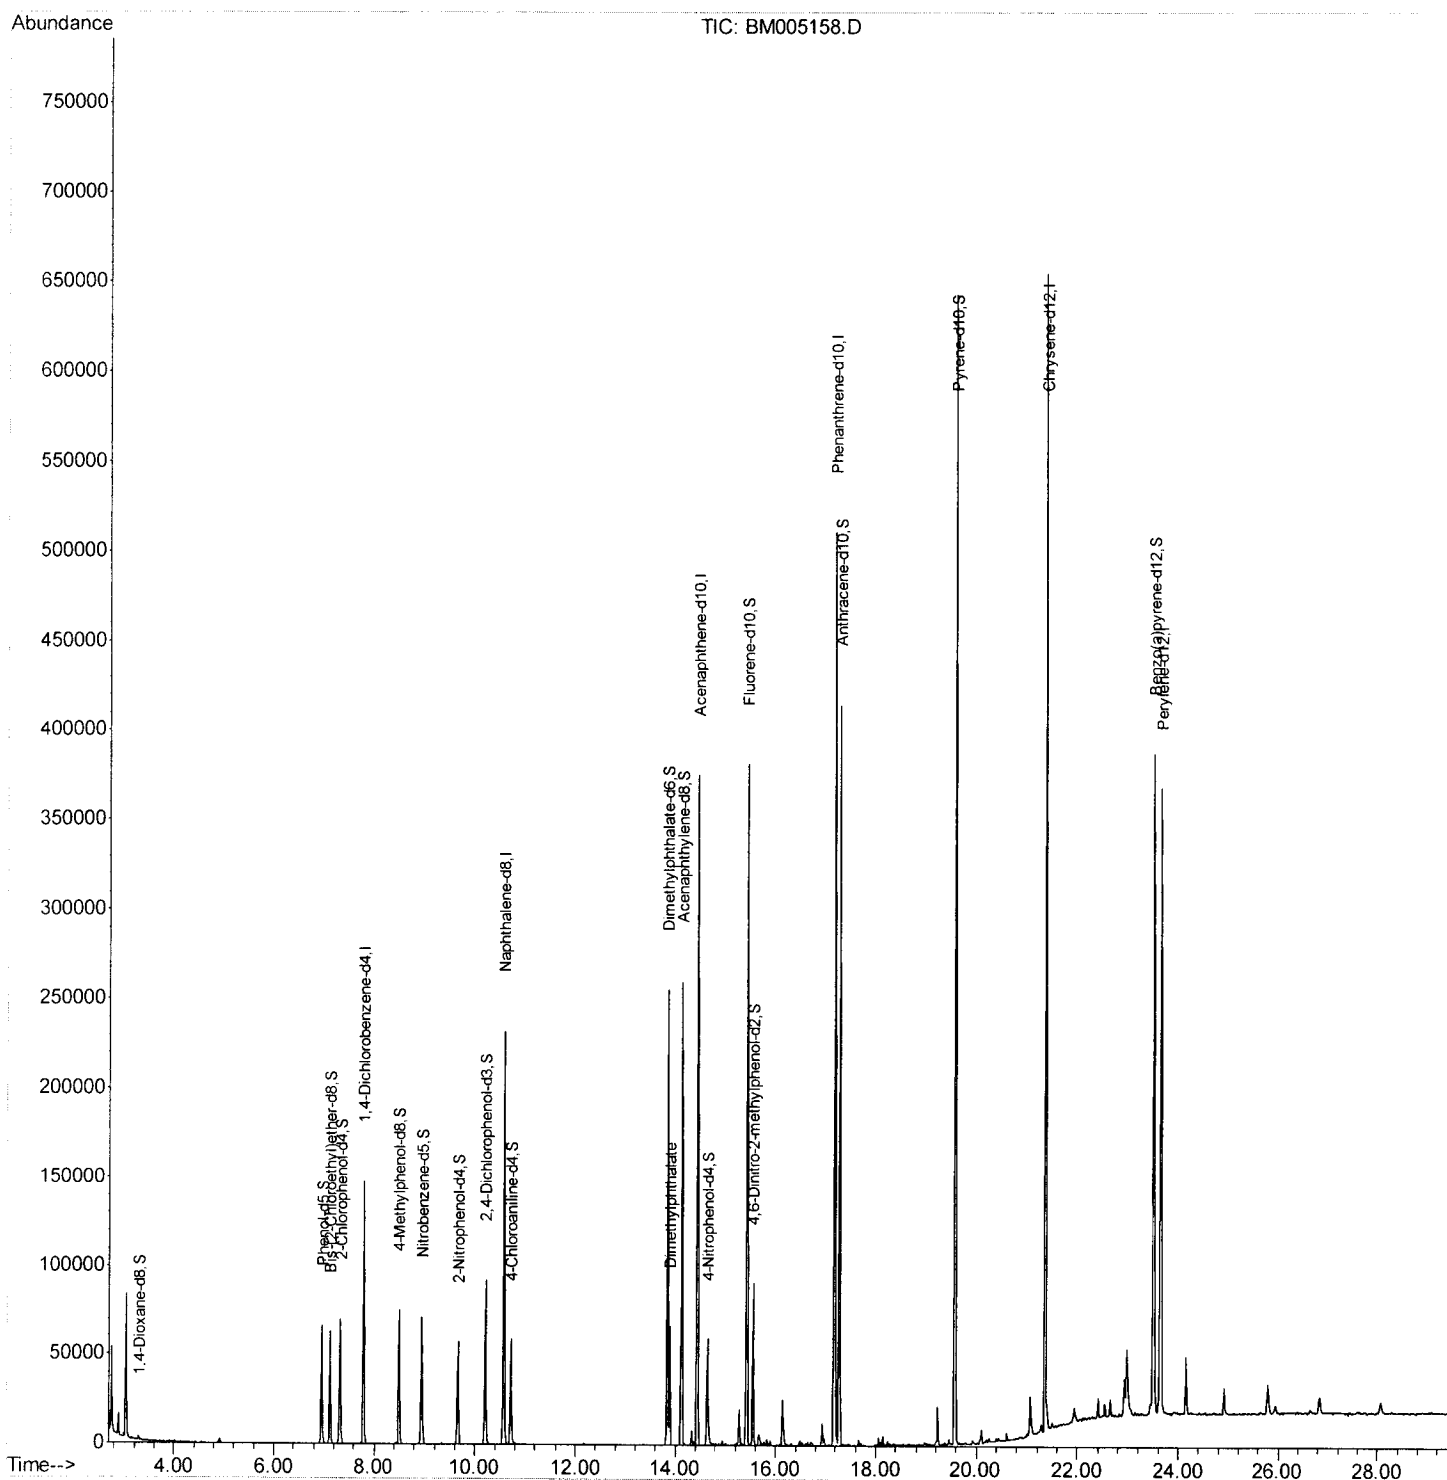

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM043016\
 Data File : BM005158.D
 Acq On : 30 Apr 2016 01:10
 Operator : UM/SJ
 Sample : H2729-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B8

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:40 AM

Quant Time: Apr 30 04:41:34 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

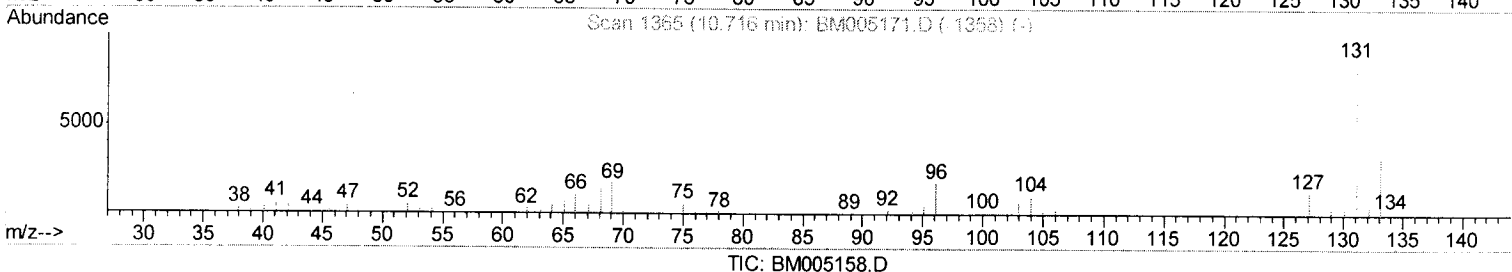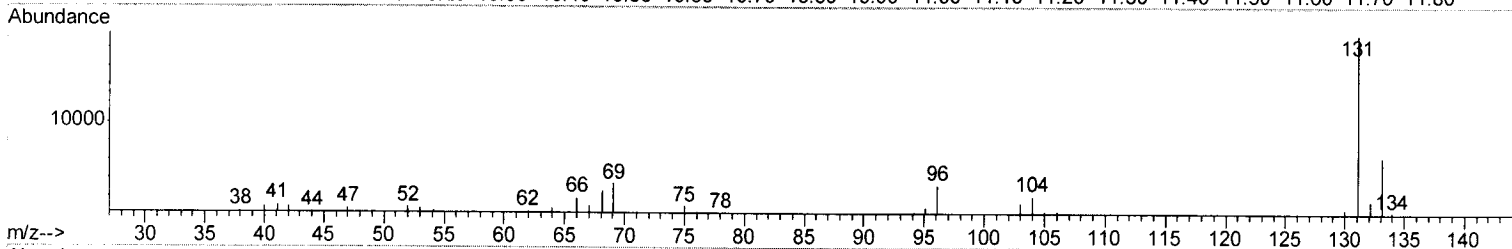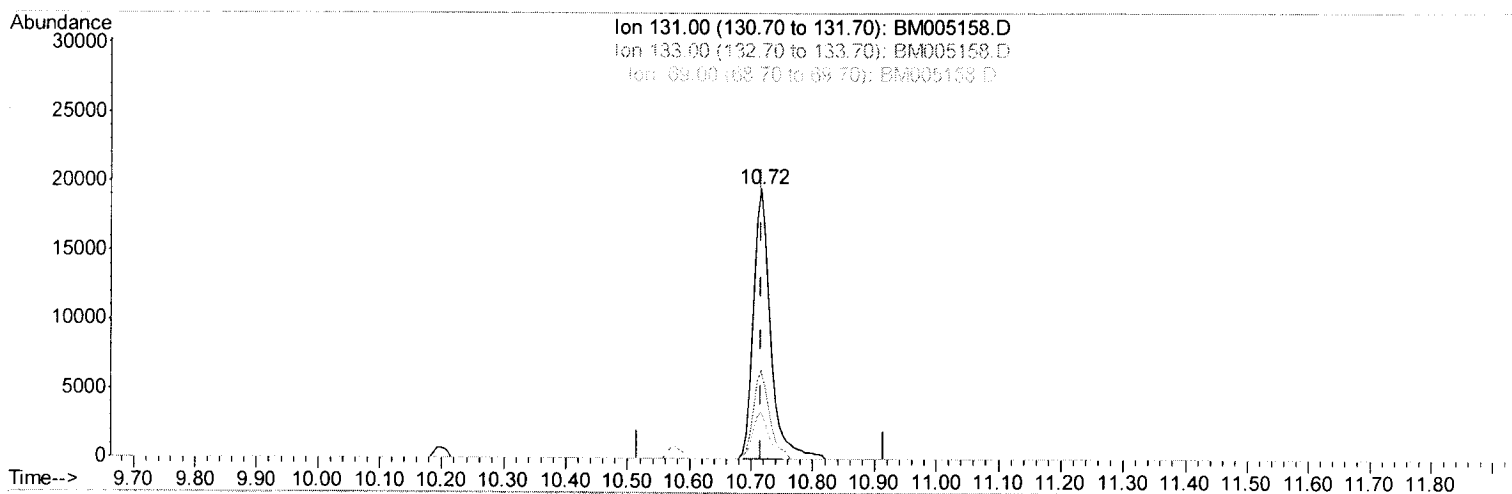

(29) 4-Chloroaniline-d4 (S)

10.716min (+0.000) 11.19ng/ul m U.M

response 37298

05/07/16

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	32.65
69.00	16.70	17.47
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM043016\
 Data File : BM005158.D
 Acq On : 30 Apr 2016 01:10
 Operator : UM/SJ
 Sample : H2729-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BD3B8

Quant Time: May 07 07:48:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
 4/30/2016 11:27:40 AM

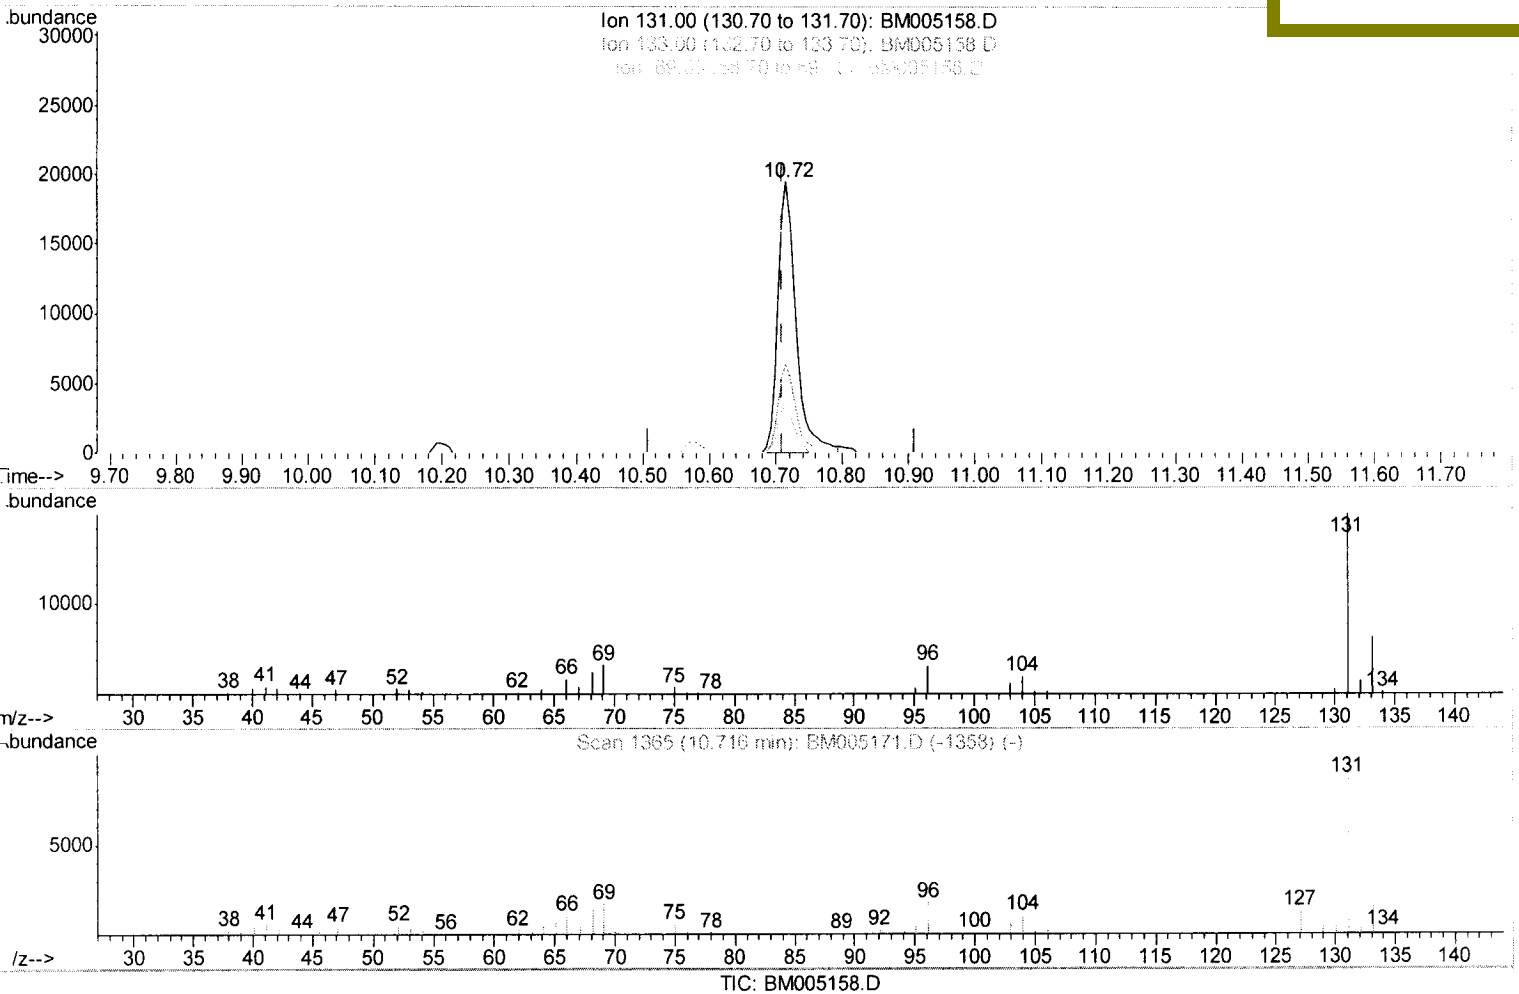

(29) 4-Chloroaniline-d4 (S)

10.716min (+0.006) 11.04ng/ul

response 36788

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	32.65
69.00	16.70	17.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM043016\
 Data File : BM005158.D
 Acq On : 30 Apr 2016 01:10
 Operator : UM/SJ
 Sample : H2729-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B8

Quant Time: Apr 30 04:41:34 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:40 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	40062	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	193742	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	126057	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	293480	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	315550	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	256464	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	1603	2.03	ng/uL	0.00
5) Phenol-d5	6.96	99	42032	12.68	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.12	67	28067	14.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	34170	13.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	31240	11.12	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	17652	13.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	19816	13.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	37225	13.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	37298m	11.19	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	167950	16.87	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	187112	15.78	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	19431	11.17	ng/ul	0.00
57) Fluorene-d10	15.42	176	148321	16.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	20178	12.09	ng/ul	0.00
70) Anthracene-d10	17.27	188	245593	18.66	ng/ul	0.00
76) Pyrene-d10	19.57	212	324058	22.56	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	255024	22.19	ng/ul	-0.01

U.M
 05/07/16

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	43150	4.32	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed