

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
 Data File : BM005155.D
 Acq On : 29 Apr 2016 22:45
 Operator : UM/SJ
 Sample : H2729-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3D8

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:36 AM

Quant Time: Apr 30 05:05:08 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	34347	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	162618	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	103645	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	240939	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	230715	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	188280	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	5194	7.68	ng/uL	0.00
5) Phenol-d5	6.96	99	112573	39.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	71711	44.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	90451	40.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	95844	39.79	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	46234	41.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	53501	42.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	93366	39.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	276873m	98.96	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	340259	41.57	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	396794	40.71	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	49389m	34.52	ng/ul	0.00
57) Fluorene-d10	15.42	176	287877	40.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	44556	32.51	ng/ul	0.00
70) Anthracene-d10	17.27	188	443452	41.05	ng/ul	0.00
76) Pyrene-d10	19.57	212	485782	46.25	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	370089	43.87	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.88	163	73270	8.93	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
Data File : BM005155.D
Acq On : 29 Apr 2016 22:45
Operator : UM/SJ
Sample : H2729-17
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BD3D8

Manual Integrations
APPROVED

sohil
4/30/2016 11:27:36 AM

Quant Time: Apr 30 05:05:08 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 30 03:07:27 2016
Response via : Initial Calibration

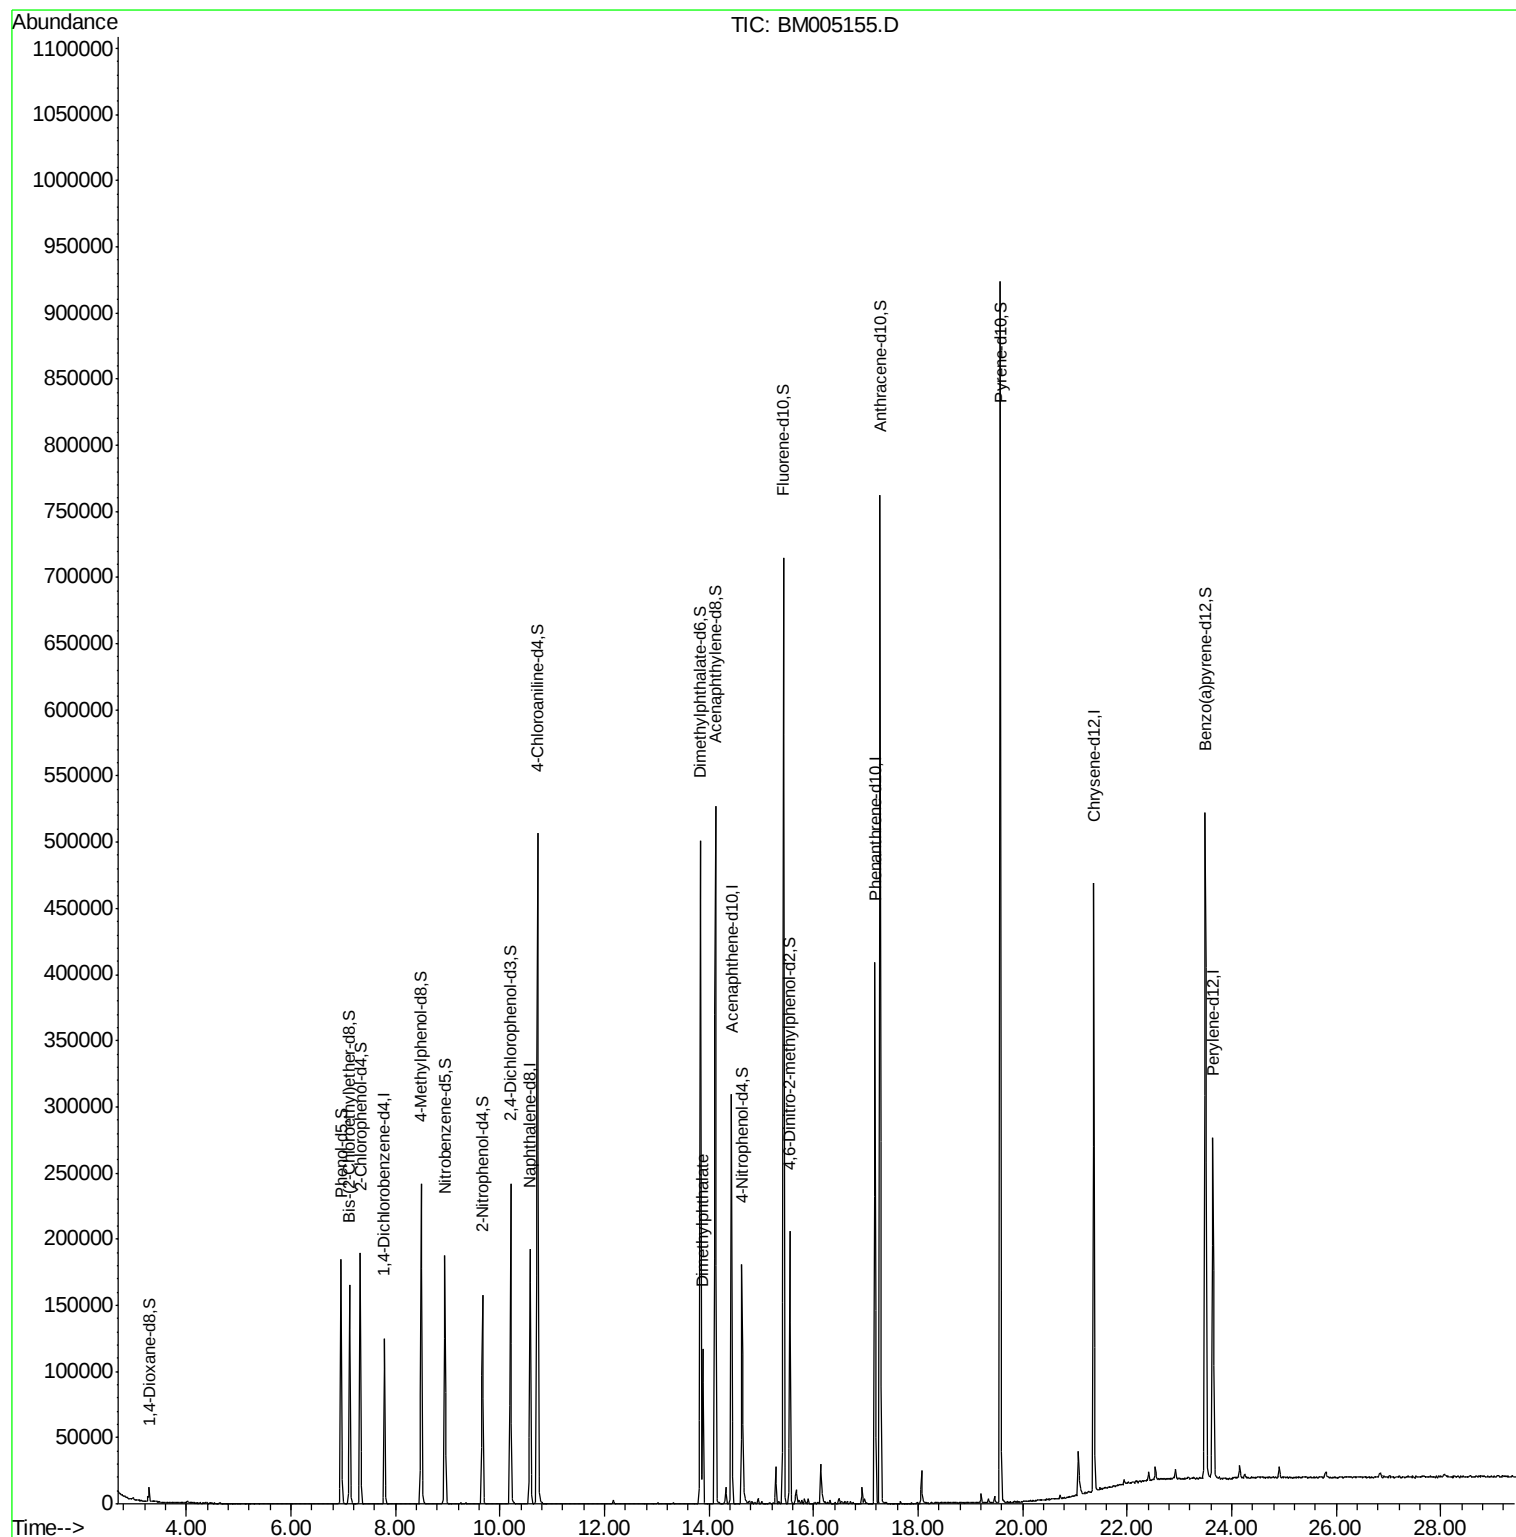

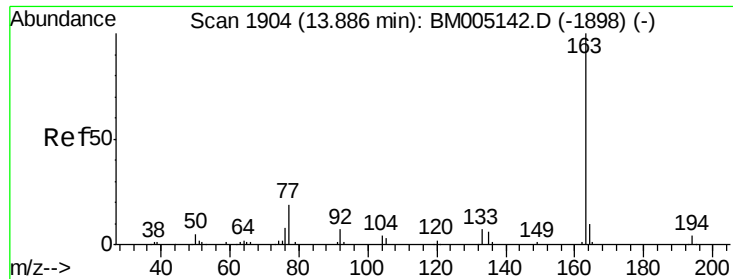


#44
 Dimethylphthalate
 Concen: 8.93 ng/ul
 RT: 13.88 min Scan# 1903
 Delta R.T. -0.01 min
 Lab File: BM005155.D
 Acq: 29 Apr 2016 22:45

Instrument :
 BNA_M
 ClientSampleId :
 BD3D8

Tot Ion:	163	Resp:	73270
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.3	4.9
164	10.0	8.2	12.2

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:36 AM

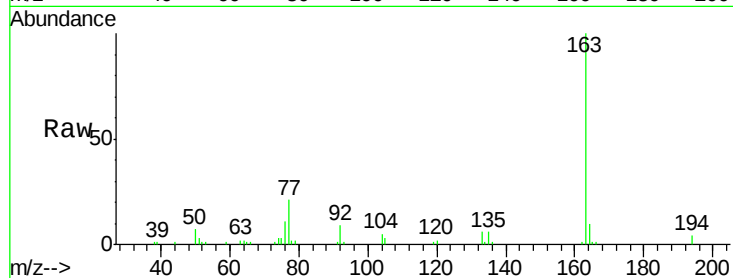

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

