

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
 Data File : BM005156.D
 Acq On : 29 Apr 2016 23:21
 Operator : UM/SJ
 Sample : H2729-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3D9

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:39 AM

Quant Time: Apr 30 05:06:37 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	34672	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	163803	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	105129	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	249849	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	275455	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	224405	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	3355	4.92	ng/uL	0.00
5) Phenol-d5	6.96	99	69158	24.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	43504	26.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	55263	24.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	56657	23.30	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	27255	24.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	30883	24.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	56089	23.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	63582m	22.56	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	217717	26.22	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	249619	25.25	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	28082m	19.35	ng/ul	0.00
57) Fluorene-d10	15.42	176	189427	25.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	26199	18.44	ng/ul	0.00
70) Anthracene-d10	17.27	188	303797	27.12	ng/ul	0.00
76) Pyrene-d10	19.57	212	358413	28.58	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	289142	28.76	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.88	163	55032	6.61	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
Data File : BM005156.D
Acq On : 29 Apr 2016 23:21
Operator : UM/SJ
Sample : H2729-18
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BD3D9

Manual Integrations
APPROVED

sohil
4/30/2016 11:27:39 AM

Quant Time: Apr 30 05:06:37 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 30 03:07:27 2016
Response via : Initial Calibration

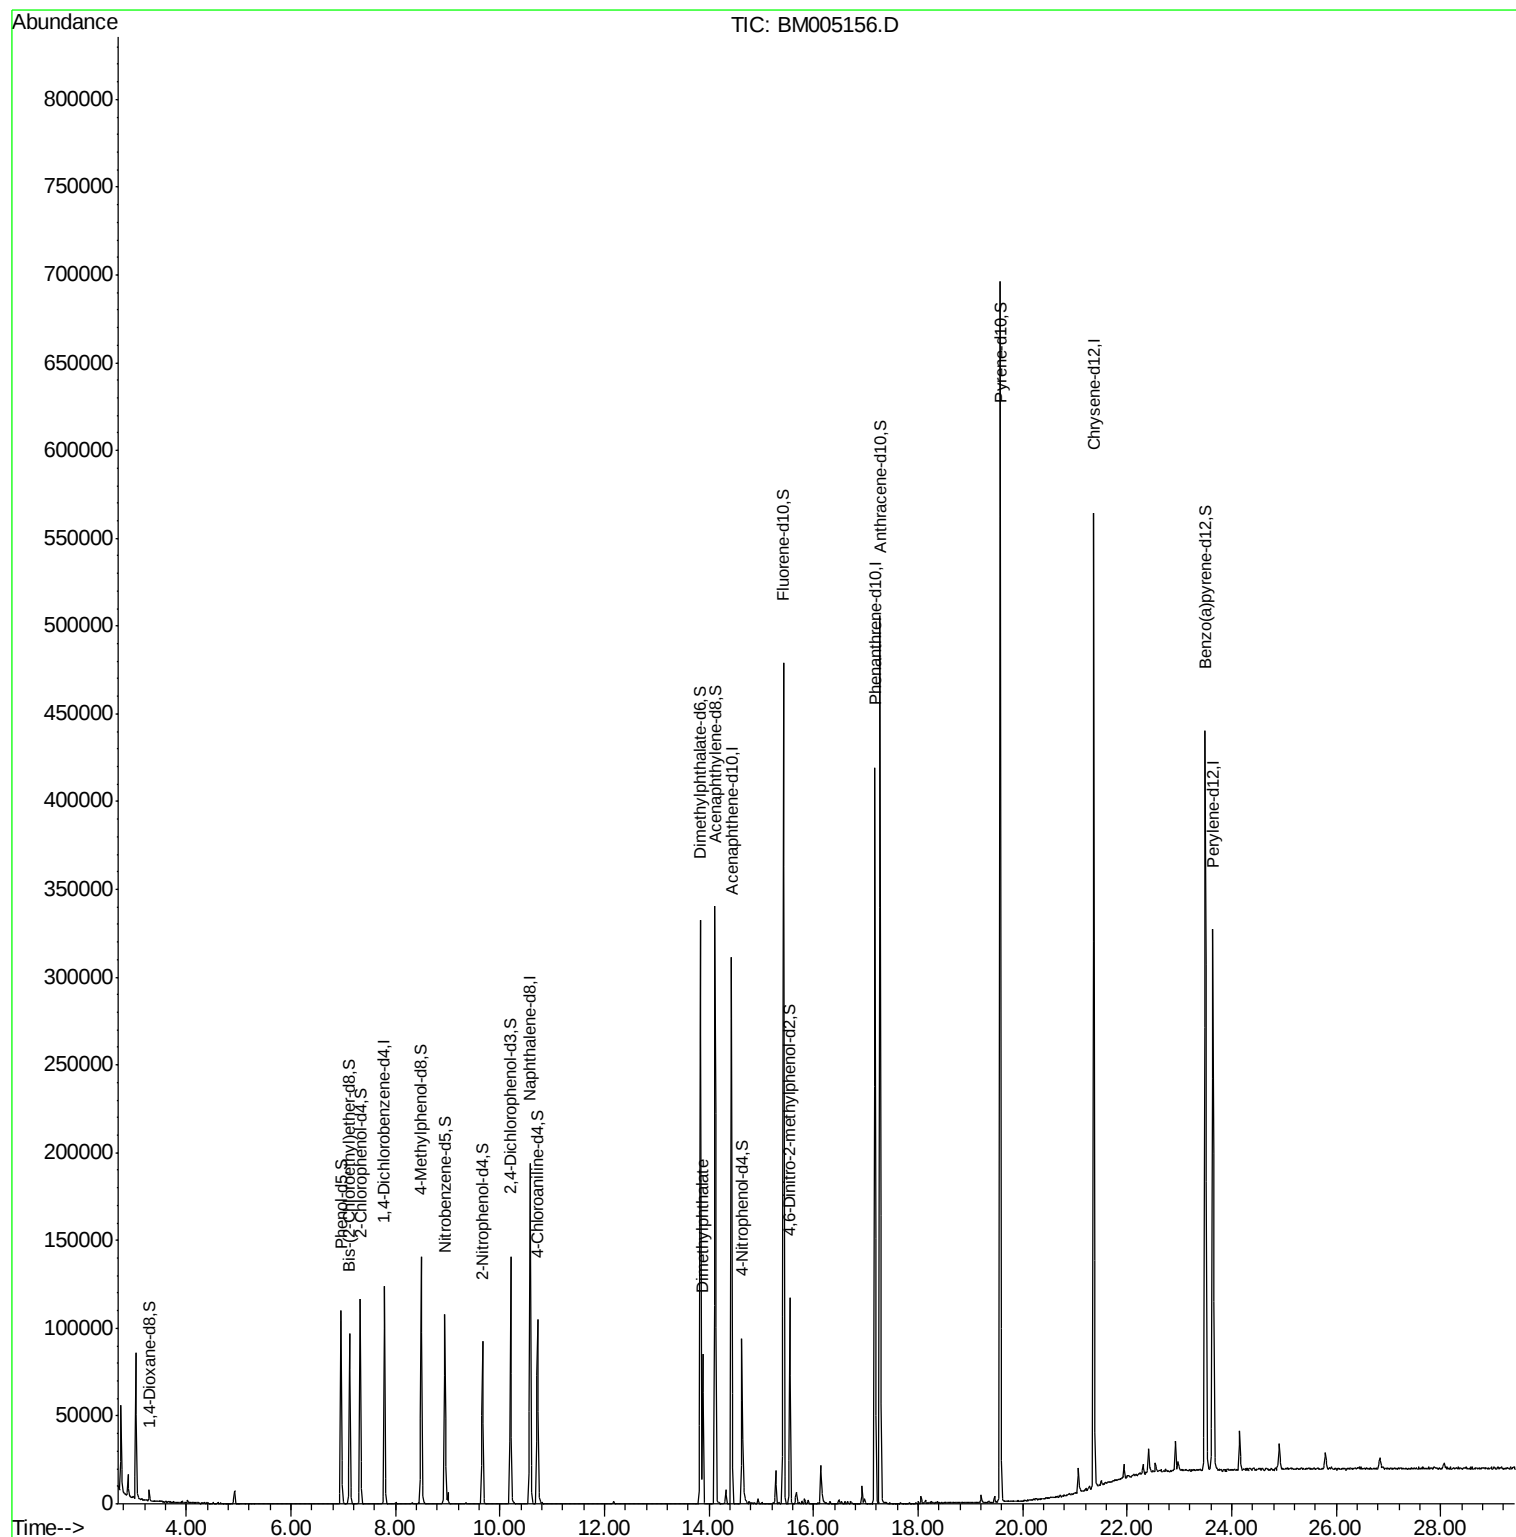

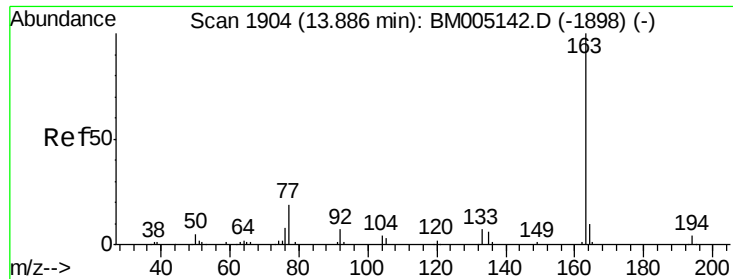


#44
 Dimethylphthalate
 Concen: 6.61 ng/ul
 RT: 13.88 min Scan# 1903
 Delta R.T. -0.01 min
 Lab File: BM005156.D
 Acq: 29 Apr 2016 23:21

Instrument :
 BNA_M
 ClientSampleId :
 BD3D9

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.3	3.3	4.9
164	10.4	8.2	12.2

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:39 AM

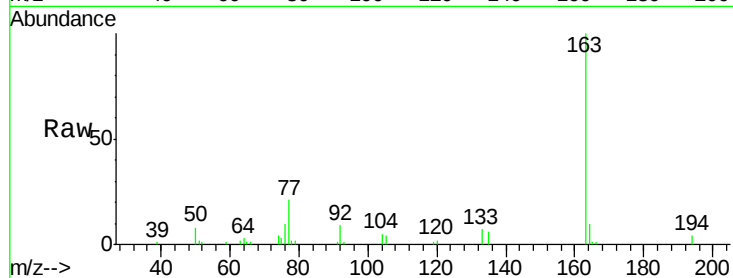

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

