

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
 Data File : BM005160.D
 Acq On : 30 Apr 2016 02:22
 Operator : UM/SJ
 Sample : H2729-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3C0

Manual Integrations
 APPROVED

sohil
 4/30/2016 11:27:42 AM

Quant Time: Apr 30 05:13:08 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	37644	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	178882	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	113927	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	265833	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	276152	20.00	ng/ul	-0.01
83) Perylene-d12	23.64	264	224305	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	5601	7.56	ng/uL	0.00
5) Phenol-d5	6.96	99	119611	38.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	74972	42.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	96373	39.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	99432	37.66	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	49103	39.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	55911	40.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	98110	37.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	103867m	33.75	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	349583	38.85	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	414353	38.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	52732m	33.53	ng/ul	0.00
57) Fluorene-d10	15.42	176	300280	37.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	48553	32.11	ng/ul	0.00
70) Anthracene-d10	17.27	188	467482	39.22	ng/ul	0.00
76) Pyrene-d10	19.57	212	527664	41.97	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	416197	41.41	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.88	163	67406	7.47	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
Data File : BM005160.D
Acq On : 30 Apr 2016 02:22
Operator : UM/SJ
Sample : H2729-09
Misc :
ALS Vial : 19 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BD3C0

Manual Integrations
APPROVED

sohil
4/30/2016 11:27:42 AM

Quant Time: Apr 30 05:13:08 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 30 03:07:27 2016
Response via : Initial Calibration

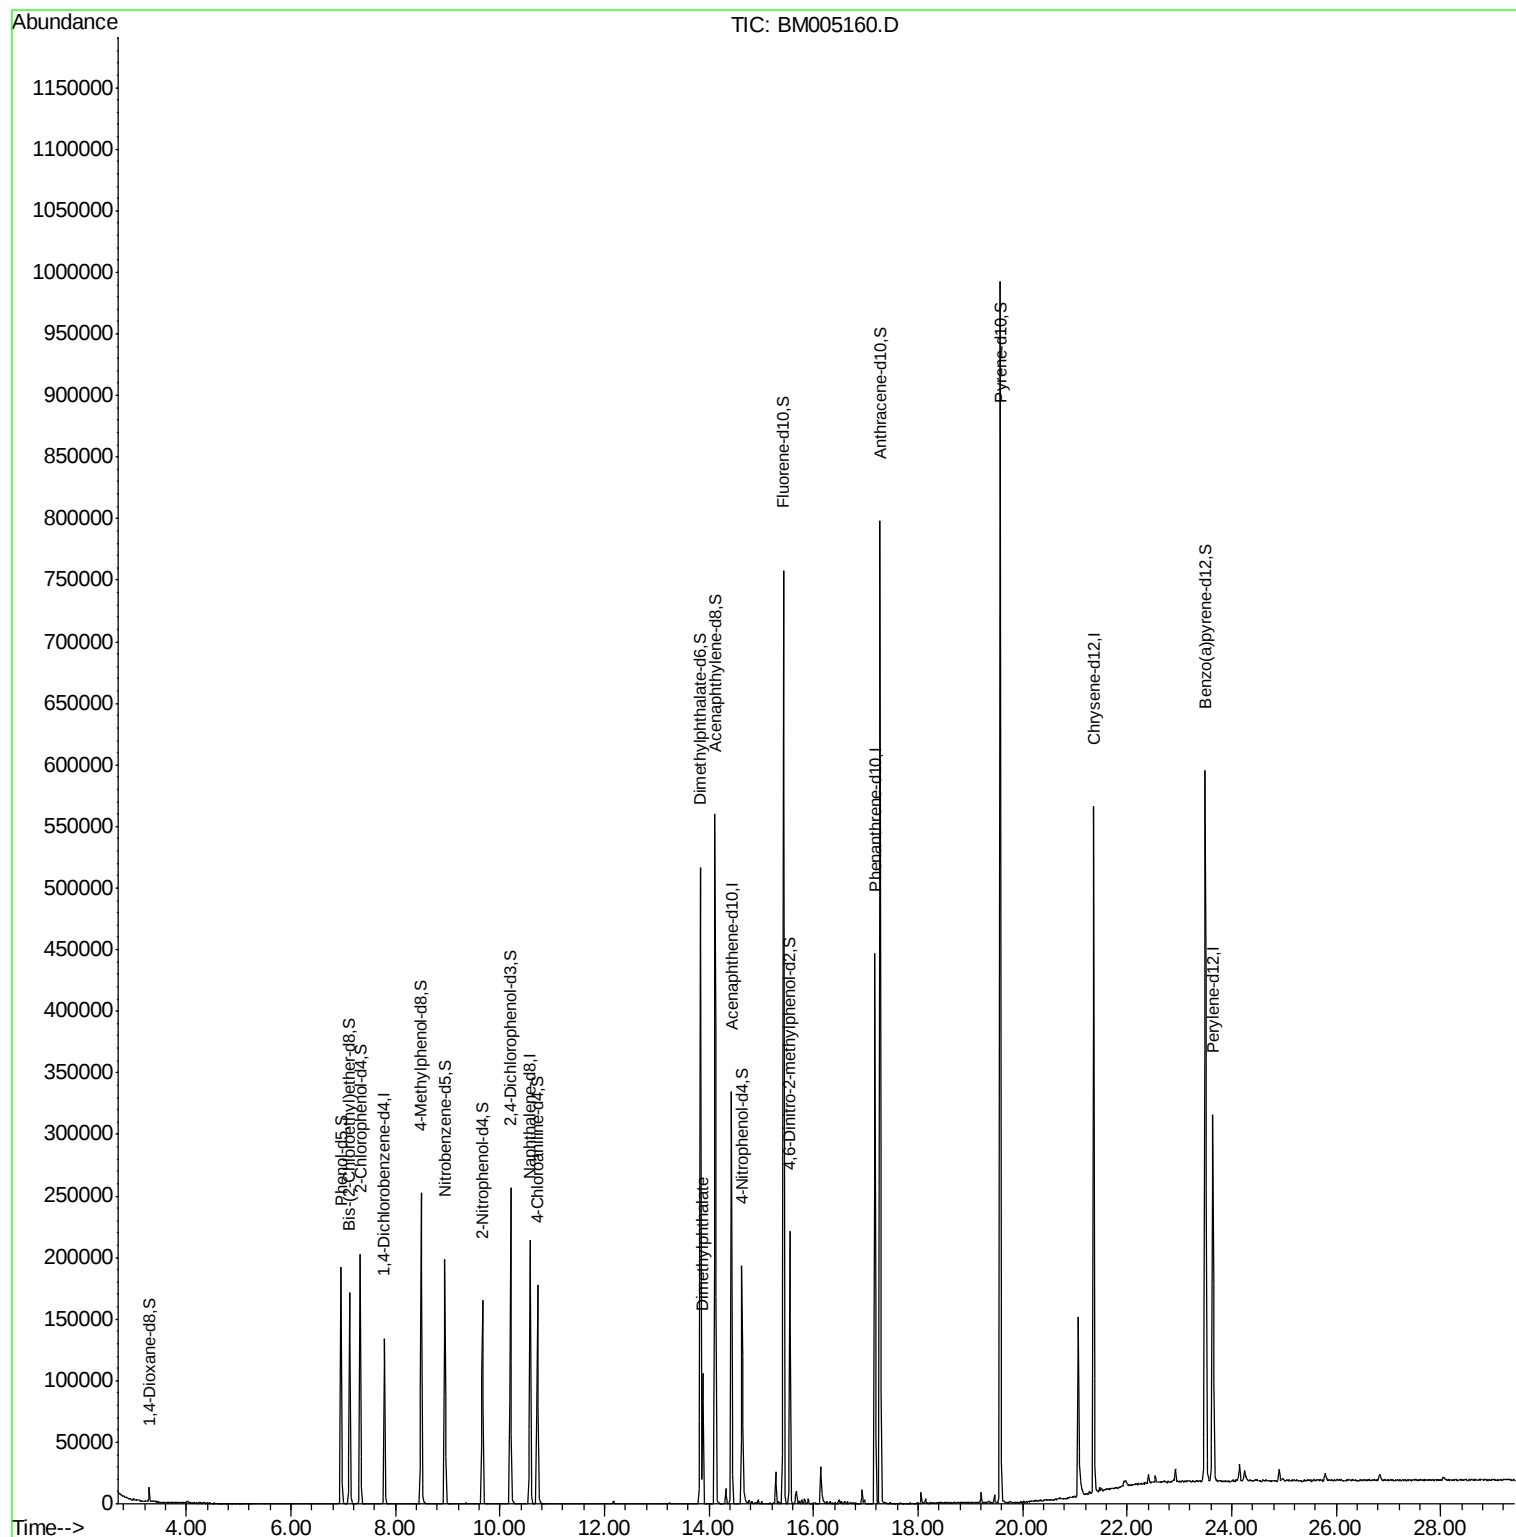

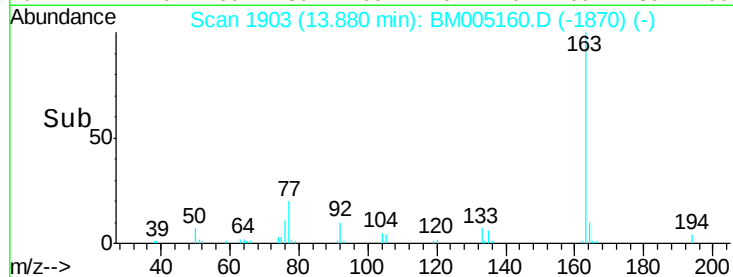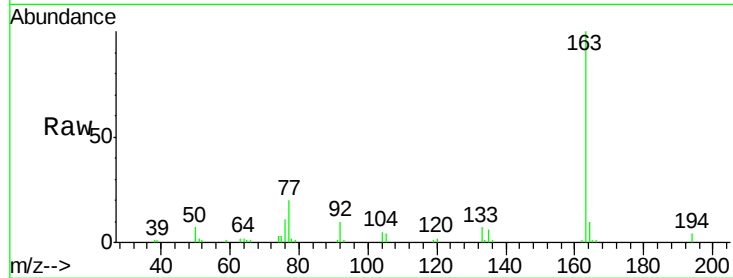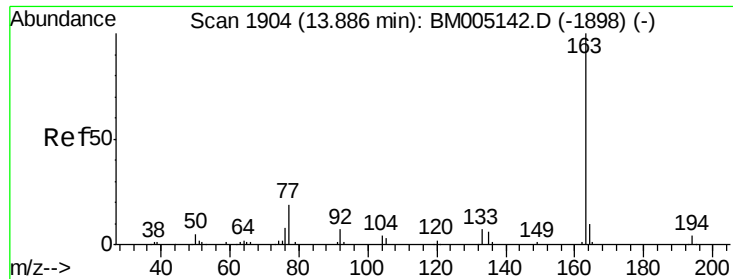

#44

Dimethylphthalate

Concen: 7.47 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. -0.01 min

Lab File: BM005160.D

Acq: 30 Apr 2016 02:22

Tot Ion:	163	Resp:	67406
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.3	4.9
164	9.7	8.2	12.2

Instrument :

BNA_M

ClientSampleId :

BD3C0

Manual Integrations
APPROVED

sohil
4/30/2016 11:27:42 AM

