

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
 Data File : BM005161.D
 Acq On : 30 Apr 2016 02:58
 Operator : UM/SJ
 Sample : H2729-11 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3D3

Quant Time: Apr 30 11:41:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	43885	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	210807	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	133260	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	305497	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	283837	20.00	ng/ul	-0.01
83) Perylene-d12	23.63	264	228999	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	741	0.86	ng/uL	0.00
5) Phenol-d5	6.96	99	17680	4.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	11628	5.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	14430	5.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	13016	4.23	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	6196	4.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	6605	4.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	14468	4.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	12171	3.36	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	53508	5.08	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	63888	5.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	2730	1.48	ng/ul	0.01
57) Fluorene-d10	15.42	176	52169	5.64	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	3012	1.73	ng/ul	0.00
70) Anthracene-d10	17.27	188	76775	5.60	ng/ul	0.00
76) Pyrene-d10	19.56	212	84076	6.51	ng/ul	-0.01
87) Benzo(a)pyrene-d12	23.49	264	57309	5.59	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	12703	1.20	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005161.D
Acq On : 30 Apr 2016 02:58
Operator : UM/SJ
Sample : H2729-11 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D3

Quant Time: Apr 30 11:41:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 30 03:07:27 2016
Response via : Initial Calibration

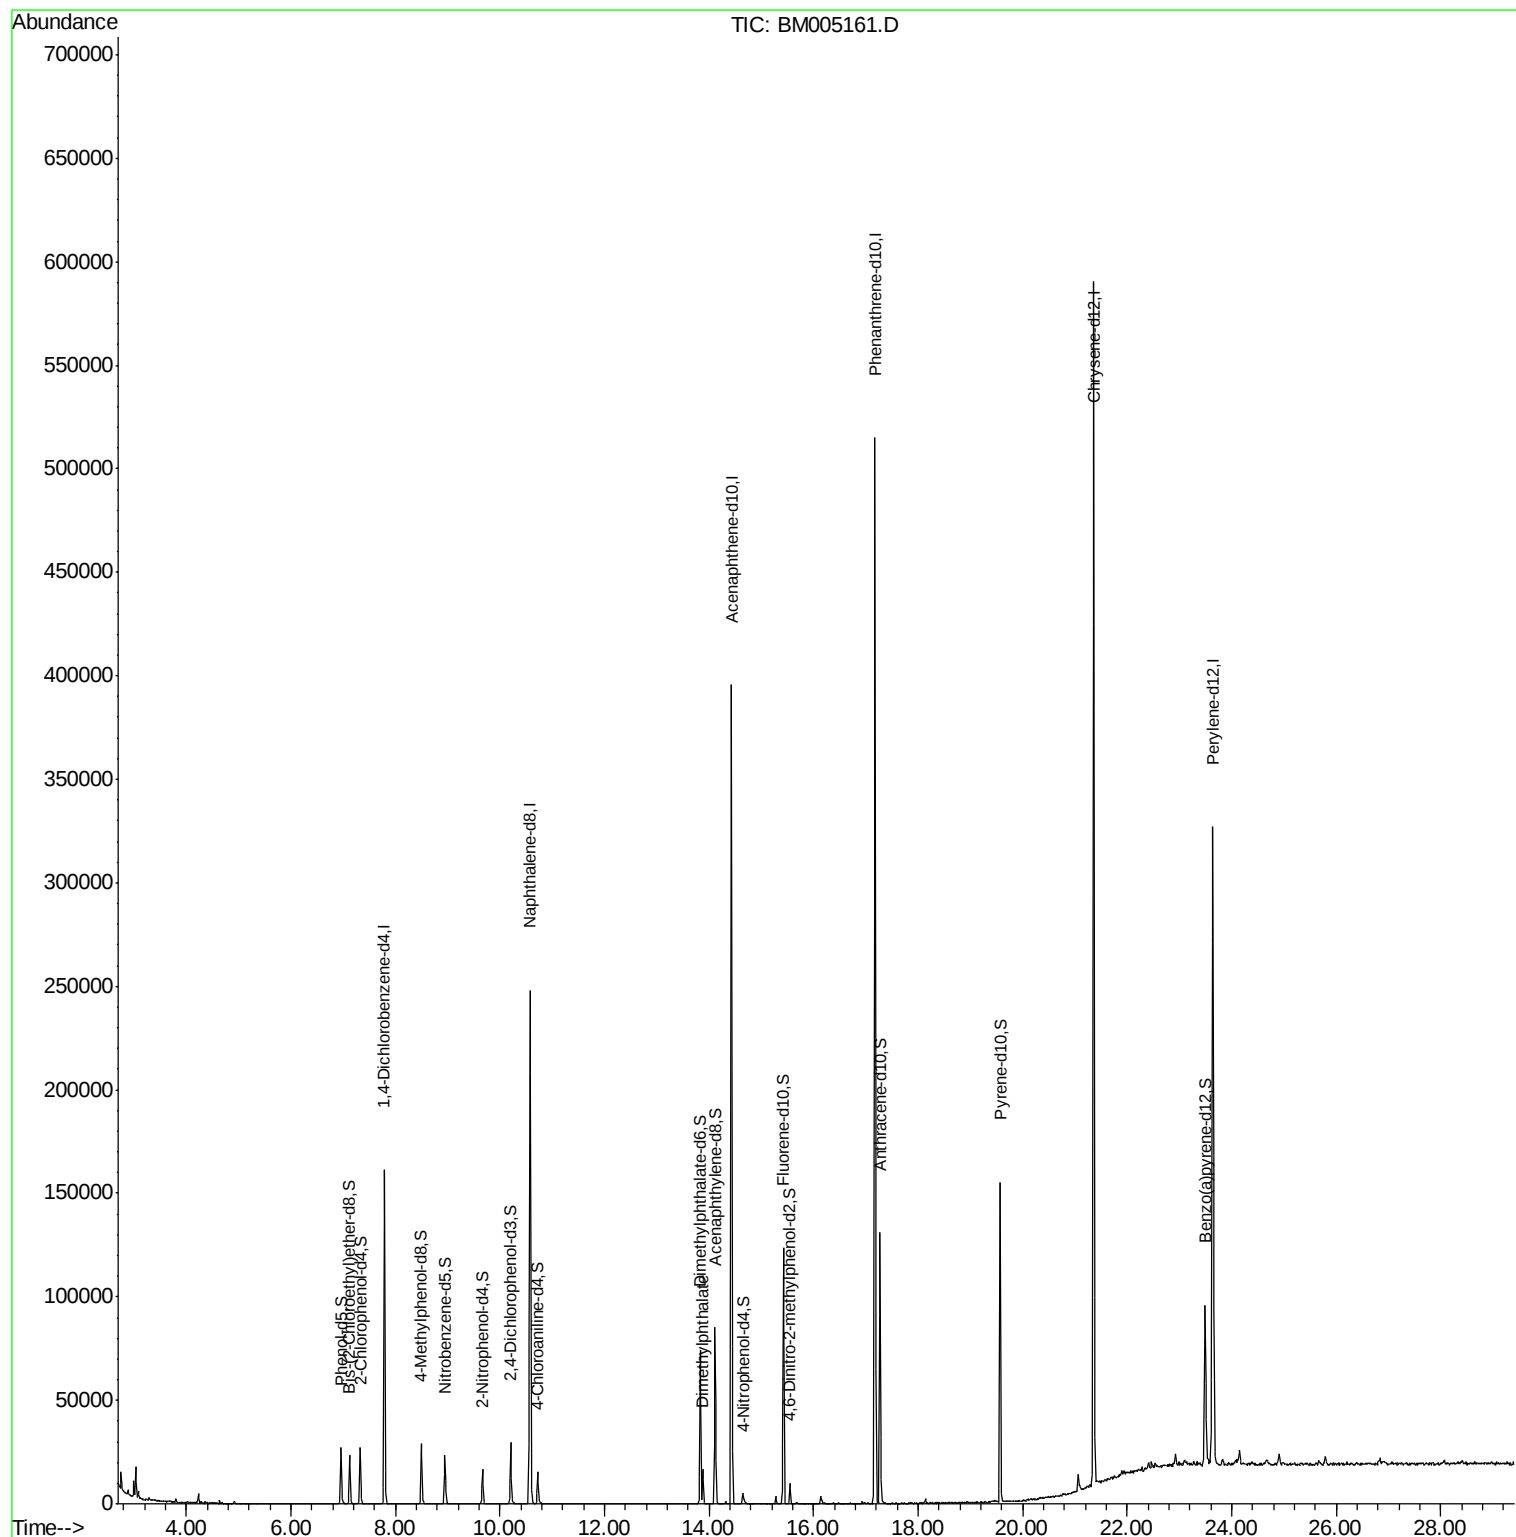

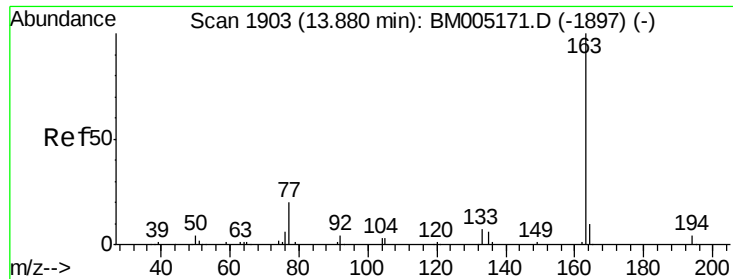

#44

Dimethylphthalate

Concen: 1.20 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. -0.01 min

Lab File: BM005161.D


Acq: 30 Apr 2016 02:58

Instrument :

BNA_M

ClientSampleId :

BD3D3

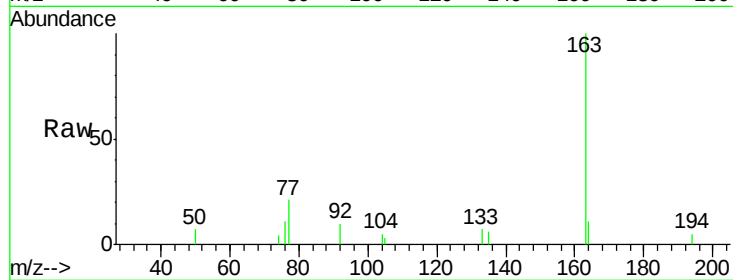

Tgt Ion:163 Resp: 12703

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9

164 10.9 8.2 12.2

