

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
 Data File : BM005168.D
 Acq On : 30 Apr 2016 10:51
 Operator : UM/SJ
 Sample : H2729-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3D3

Quant Time: Apr 30 11:44:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 30 03:07:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	43226	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	200503	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	121270	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	273925	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	258780	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	199080	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	3441	4.05	ng/uL	0.00
5) Phenol-d5	6.96	99	83266	23.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	48767	23.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	65908	23.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	63988	21.11	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	31668	22.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	34730	22.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	67636	22.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	57589	16.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	215169	22.47	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	265773	23.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	26820	16.02	ng/ul	0.00
57) Fluorene-d10	15.42	176	192982	22.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	22459	14.41	ng/ul	0.00
70) Anthracene-d10	17.27	188	293123	23.86	ng/ul	0.00
76) Pyrene-d10	19.57	212	321879	27.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	212179	23.79	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	50976	5.31	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005168.D
Acq On : 30 Apr 2016 10:51
Operator : UM/SJ
Sample : H2729-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D3

Quant Time: Apr 30 11:44:18 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 30 03:07:27 2016
Response via : Initial Calibration

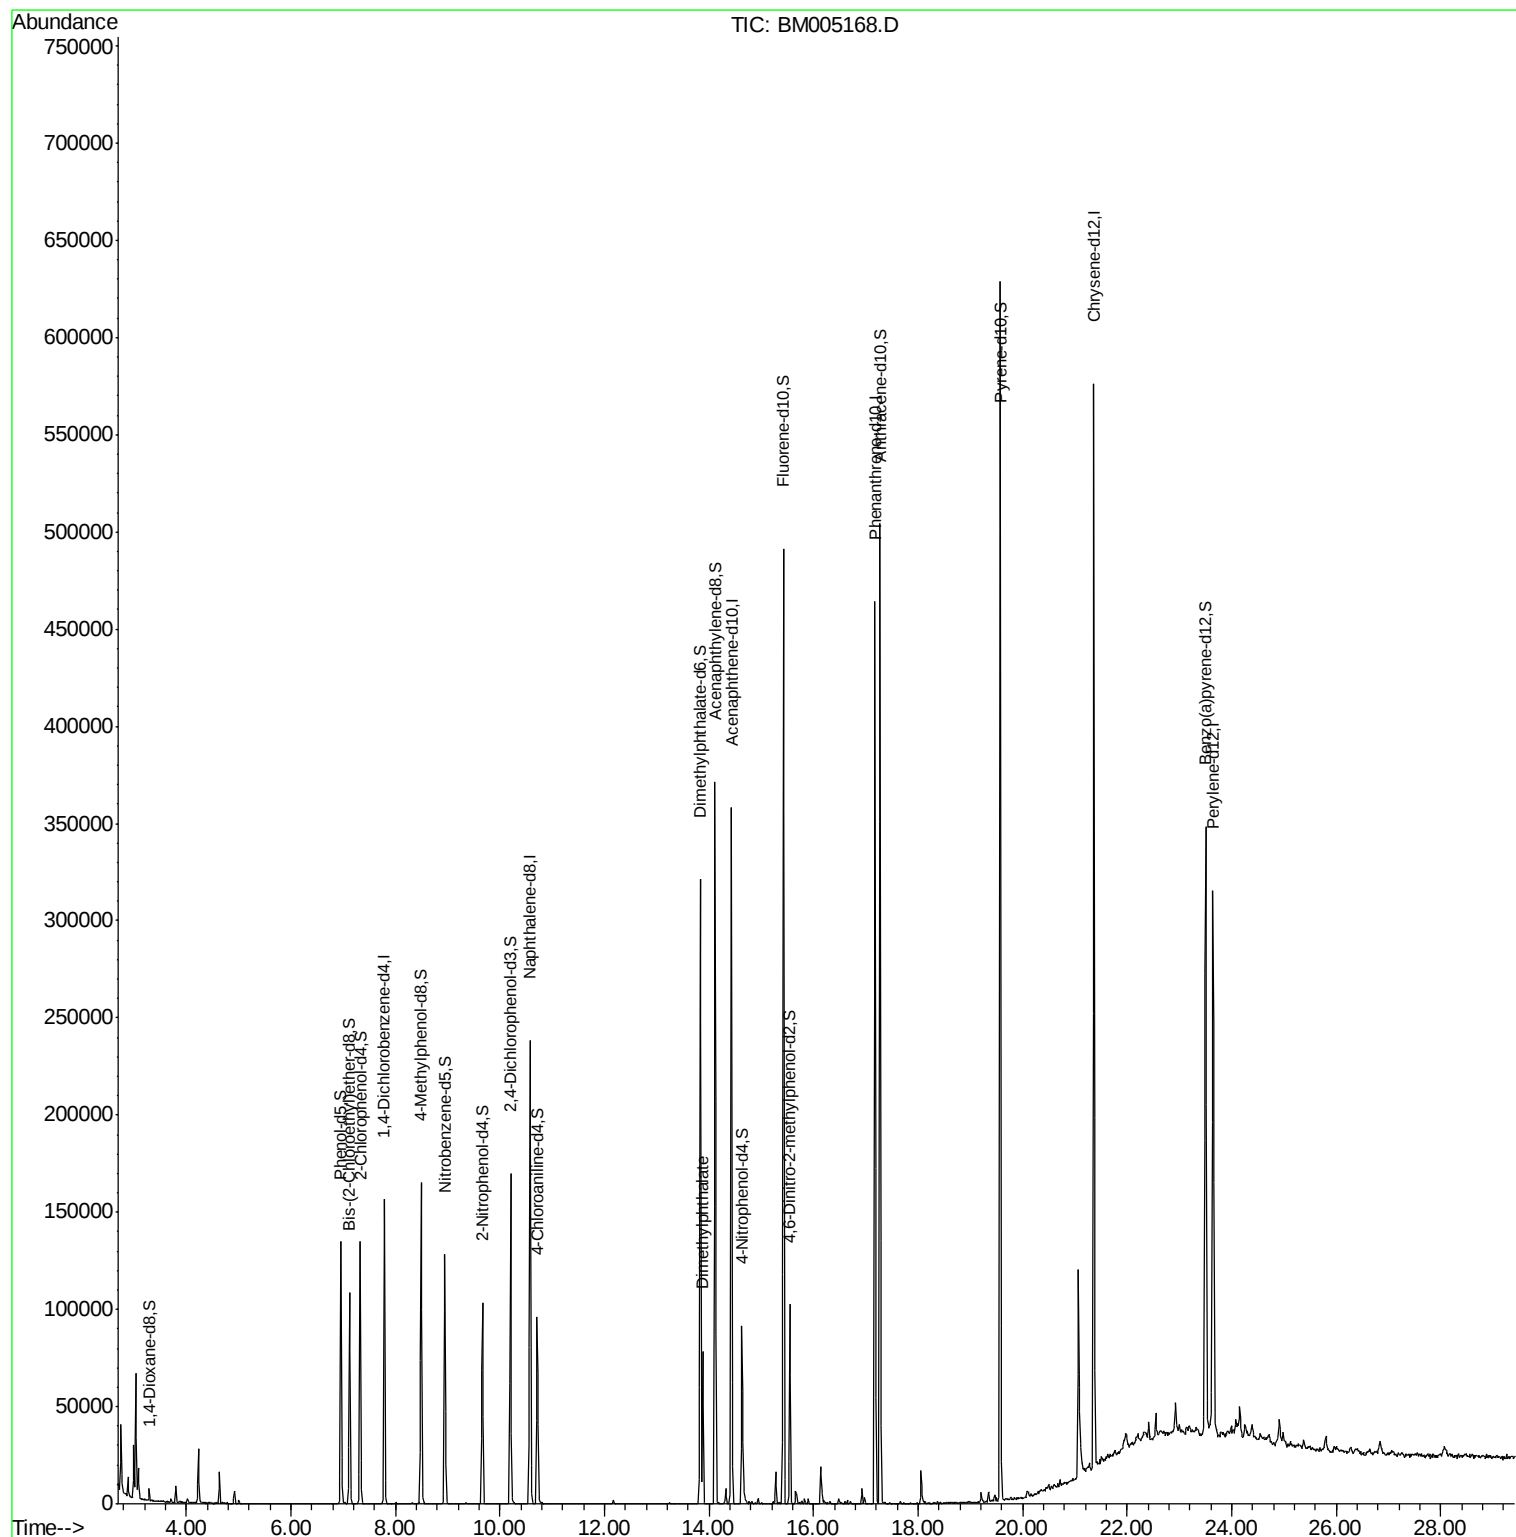

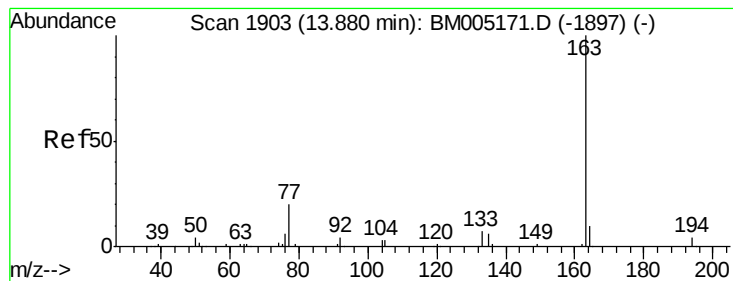

#44

Dimethylphthalate

Concen: 5.31 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. -0.01 min

Lab File: BM005168.D


Acq: 30 Apr 2016 10:51

Instrument :

BNA_M

ClientSampleId :

BD3D3

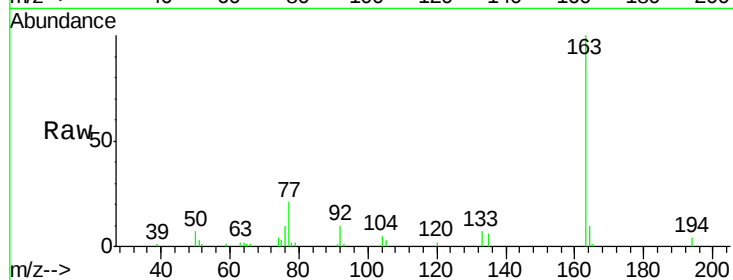


Tgt Ion:163 Resp: 50976

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 9.9 8.2 12.2

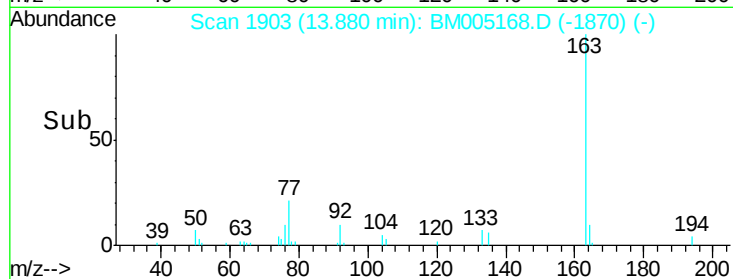

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

