

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
 Data File : BM005146.D
 Acq On : 29 Apr 2016 17:18
 Operator : UM/SJ
 Sample : H2778-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.957	721	726	735	rBV	39239	59286	4.48%	0.547%
2	7.122	748	754	766	rBB	142046	215456	16.28%	1.988%
3	7.322	782	788	799	rBB	137948	216324	16.35%	1.996%
4	7.787	861	867	876	rBB	127462	201259	15.21%	1.857%
5	8.492	981	987	999	rBB	113578	178740	13.51%	1.650%
6	8.945	1058	1064	1075	rBV	162590	268385	20.28%	2.477%
7	9.663	1180	1186	1196	rBB	143234	222433	16.81%	2.053%
8	10.198	1271	1277	1290	rBV	199125	334637	25.29%	3.088%
9	10.575	1335	1341	1352	rVB	207939	341491	25.81%	3.152%
10	13.833	1889	1895	1908	rBB	474120	649762	49.11%	5.997%
11	14.122	1937	1944	1959	rBV	496934	751079	56.77%	6.932%
12	14.427	1990	1996	2003	rBB2	330567	510883	38.61%	4.715%
13	14.639	2027	2032	2041	rBV	21157	37592	2.84%	0.347%
14	15.421	2159	2165	2174	rBB	694372	992678	75.03%	9.161%
15	15.545	2181	2186	2193	rBV	199431	263248	19.90%	2.430%
16	17.174	2457	2463	2474	rBV	452670	635833	48.06%	5.868%
17	17.274	2474	2480	2490	rBV2	780630	1119536	84.61%	10.332%
18	19.568	2864	2870	2884	rBV2	916403	1323121	100.00%	12.211%
19	21.362	3170	3175	3182	rBV	588810	747982	56.53%	6.903%
20	22.209	3315	3319	3324	rVB	14951	16116	1.22%	0.149%
21	22.927	3437	3441	3445	rVB	11106	15030	1.14%	0.139%
22	23.497	3530	3538	3551	rBV2	569619	1075271	81.27%	9.924%
23	23.644	3555	3563	3575	rVB2	311496	606226	45.82%	5.595%
24	24.156	3646	3650	3657	rVB	16302	27631	2.09%	0.255%
25	24.909	3774	3778	3785	rVB3	13072	25386	1.92%	0.234%


Sum of corrected areas: 10835385

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
Data File : BM005146.D
Acq On : 29 Apr 2016 17:18
Operator : UM/SJ
Sample : H2778-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B59

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

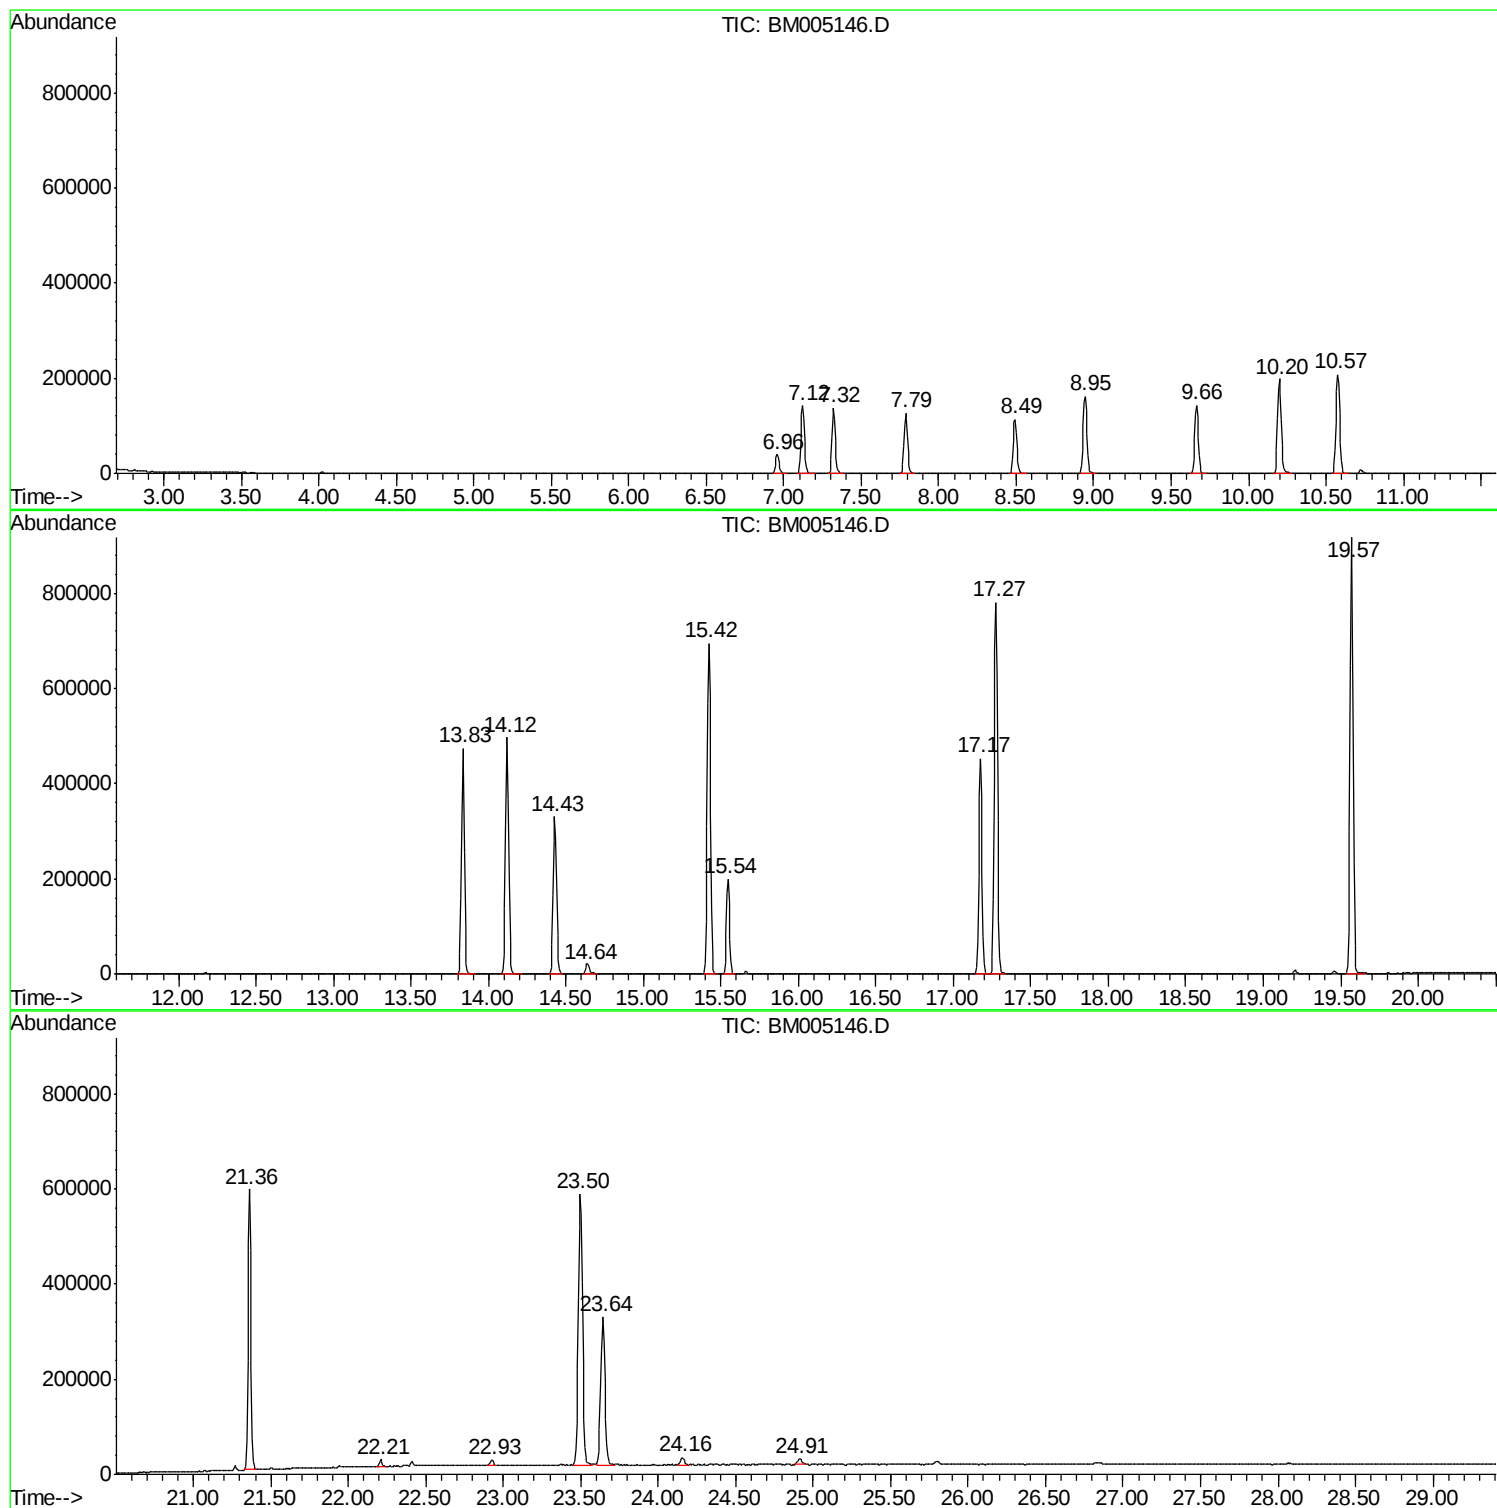

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005146.D
Acq On : 29 Apr 2016 17:18
Operator : UM/SJ
Sample : H2778-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005146.D
Acq On : 29 Apr 2016 17:18
Operator : UM/SJ
Sample : H2778-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B59

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc