

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
 Data File : BM005152.D
 Acq On : 29 Apr 2016 20:56
 Operator : UM/SJ
 Sample : H2729-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3D4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	99	102	107	rVB	10113	11606	1.03%	0.107%
2	6.957	720	726	738	rBV	172273	275805	24.44%	2.535%
3	7.122	748	754	765	rBB	152093	232316	20.58%	2.135%
4	7.322	782	788	800	rBB	178422	281937	24.98%	2.592%
5	7.787	861	867	876	rBB	103354	166546	14.76%	1.531%
6	8.492	981	987	1001	rVB	214684	352019	31.19%	3.236%
7	8.945	1058	1064	1076	rBB	171256	277331	24.57%	2.549%
8	9.663	1180	1186	1195	rBB	142944	227509	20.16%	2.091%
9	10.198	1271	1277	1292	rBB	214716	359558	31.86%	3.305%
10	10.575	1334	1341	1351	rBB	167895	270785	23.99%	2.489%
11	10.716	1359	1365	1384	rBV	179928	313375	27.76%	2.880%
12	13.833	1889	1895	1900	rBV	433452	592089	52.46%	5.442%
13	13.880	1900	1903	1910	rVB	107792	136125	12.06%	1.251%
14	14.116	1937	1943	1959	rBV	459733	704810	62.44%	6.479%
15	14.427	1990	1996	2003	rBB2	241289	372098	32.97%	3.420%
16	14.627	2026	2030	2050	rBV	148035	243924	21.61%	2.242%
17	15.268	2135	2139	2144	rVB	20217	25277	2.24%	0.232%
18	15.421	2159	2165	2173	rBV	617721	892318	79.06%	8.202%
19	15.545	2181	2186	2195	rBB	175209	238973	21.17%	2.197%
20	15.663	2202	2206	2213	rBV3	8134	16628	1.47%	0.153%
21	16.133	2282	2286	2294	rBV	24012	38431	3.40%	0.353%
22	16.927	2416	2421	2425	rBV	10581	12955	1.15%	0.119%
23	17.174	2457	2463	2470	rBV	321137	449707	39.84%	4.134%
24	17.274	2473	2480	2492	rVV	650028	957361	84.82%	8.800%
25	18.062	2609	2614	2624	rVB3	20915	27064	2.40%	0.249%
26	19.568	2864	2870	2884	rBV	807605	1128706	100.00%	10.375%
27	21.062	3120	3124	3134	rBV2	29452	52723	4.67%	0.485%
28	21.362	3170	3175	3184	rBV	426003	546039	48.38%	5.019%
29	22.927	3437	3441	3444	rVB2	9234	12144	1.08%	0.112%
30	23.497	3530	3538	3548	rBV2	591598	1100906	97.54%	10.119%
31	23.639	3555	3562	3572	rBV2	264880	510361	45.22%	4.691%
32	24.156	3646	3650	3657	rVB	14993	25811	2.29%	0.237%
33	24.915	3774	3779	3786	rVB3	13057	25957	2.30%	0.239%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
Data File : BM005152.D
Acq On : 29 Apr 2016 20:56
Operator : UM/SJ
Sample : H2729-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Title : SVOA CALIBRATION


Sum of corrected areas: 10879194

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043016\
Data File : BM005152.D
Acq On : 29 Apr 2016 20:56
Operator : UM/SJ
Sample : H2729-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

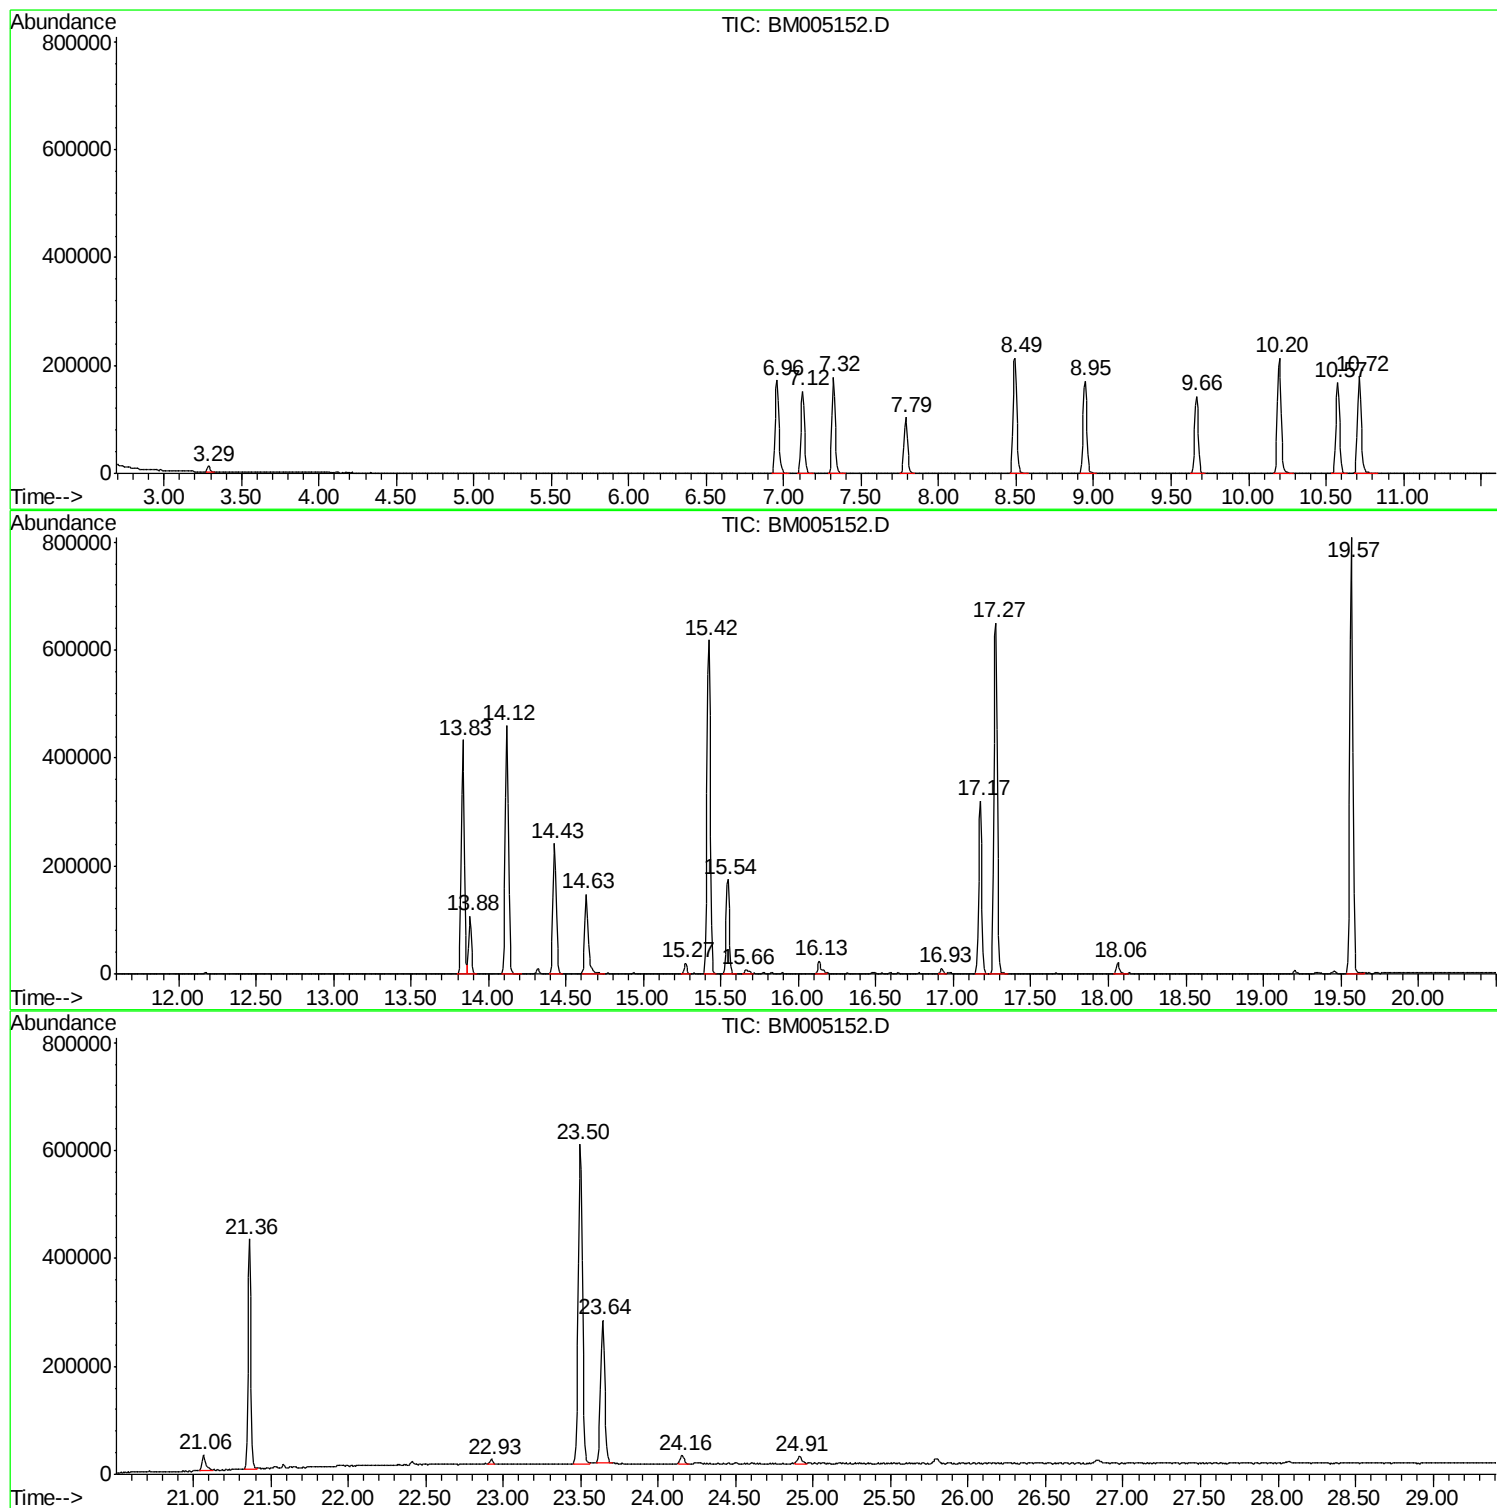

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005152.D
Acq On : 29 Apr 2016 20:56
Operator : UM/SJ
Sample : H2729-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005152.D
Acq On : 29 Apr 2016 20:56
Operator : UM/SJ
Sample : H2729-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
