

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
 Data File : BM005161.D
 Acq On : 30 Apr 2016 02:58
 Operator : UM/SJ
 Sample : H2729-11 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3D3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.752	8	11	21	rVB	9845	13636	1.81%	0.289%
2	2.993	49	52	55	rBV	7715	8271	1.10%	0.175%
3	3.028	55	58	64	rVB	15047	18553	2.46%	0.393%
4	6.957	721	726	736	rBB	26992	40258	5.34%	0.854%
5	7.122	749	754	762	rBB	23547	36468	4.84%	0.773%
6	7.322	783	788	795	rBB	27430	40964	5.43%	0.869%
7	7.787	861	867	877	rBB	161192	252414	33.48%	5.352%
8	8.492	982	987	996	rBB	29192	45221	6.00%	0.959%
9	8.945	1059	1064	1072	rBB	23285	38521	5.11%	0.817%
10	9.663	1182	1186	1192	rBB	16691	24403	3.24%	0.517%
11	10.198	1273	1277	1287	rBV	29530	48269	6.40%	1.023%
12	10.575	1334	1341	1354	rBB	248121	417524	55.38%	8.853%
13	10.716	1361	1365	1377	rBB	15345	26051	3.46%	0.552%
14	13.833	1890	1895	1899	rBV	74493	101151	13.42%	2.145%
15	13.880	1899	1903	1908	rVB	16630	22093	2.93%	0.468%
16	14.116	1938	1943	1953	rBB	85337	121981	16.18%	2.586%
17	14.427	1990	1996	2004	rBB2	395882	604910	80.23%	12.826%
18	14.645	2029	2033	2041	rBV2	5049	9441	1.25%	0.200%
19	15.421	2158	2165	2172	rBB	123451	177892	23.60%	3.772%
20	15.545	2182	2186	2190	rVB	10093	12300	1.63%	0.261%
21	17.174	2457	2463	2471	rBV	514811	737188	97.78%	15.631%
22	17.268	2474	2479	2492	rVB2	130833	182459	24.20%	3.869%
23	19.568	2864	2870	2880	rBV	154563	213726	28.35%	4.532%
24	21.062	3120	3124	3130	rBV2	8207	13895	1.84%	0.295%
25	21.356	3169	3174	3182	rBV	581941	753924	100.00%	15.986%
26	22.921	3436	3440	3444	rVB5	5764	8732	1.16%	0.185%
27	23.486	3530	3536	3545	rBV2	76546	147760	19.60%	3.133%
28	23.633	3554	3561	3573	rVB	307475	598264	79.35%	12.685%


Sum of corrected areas: 4716269

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005161.D
Acq On : 30 Apr 2016 02:58
Operator : UM/SJ
Sample : H2729-11 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BD3D3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

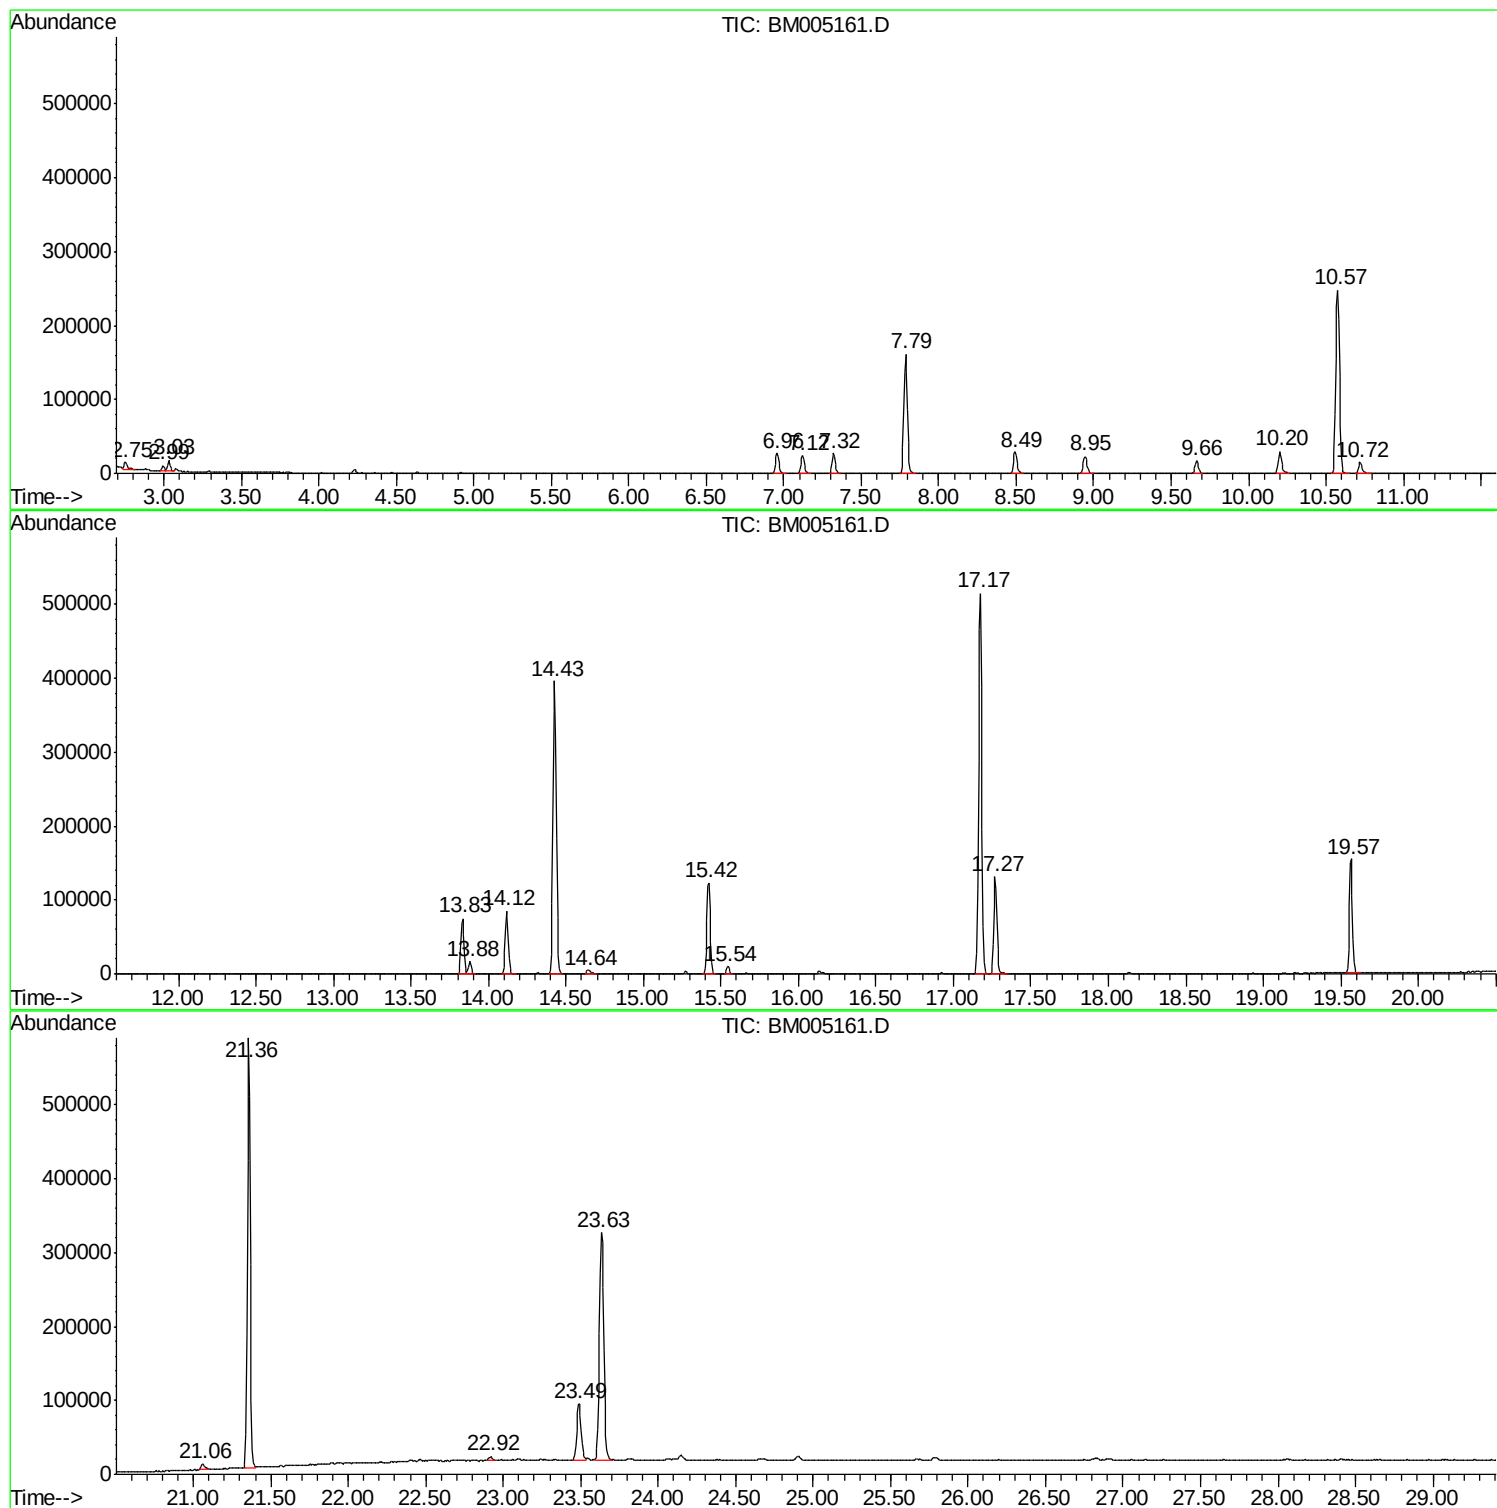

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005161.D
Acq On : 30 Apr 2016 02:58
Operator : UM/SJ
Sample : H2729-11 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM043016\
Data File : BM005161.D
Acq On : 30 Apr 2016 02:58
Operator : UM/SJ
Sample : H2729-11 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3D3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc