

Data File : BG026792.D
Acq On : 1 May 2017 3:28
Operator : SJ/MA
Sample : I2846-15
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSR8

Quant Time: May 01 05:04:03 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	183823	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	908848	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	527910	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	1020096	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	931095	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	961363	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.43	96	24526	6.01	ng/uL	0.00
5) Phenol-d5	7.18	99	559594	34.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	329752	34.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	454769	32.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	491545	36.10	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	255904	33.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	284086	34.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	432499	32.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	697655	39.70	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1388159	32.67	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1791781	33.57	ng/ul	0.00
51) 4-Nitrophenol-d4	14.83	143	253932	33.16	ng/ul	0.00
57) Fluorene-d10	15.61	176	1211288	32.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	194149	31.34	ng/ul	0.00
70) Anthracene-d10	17.45	188	1651396	33.36	ng/ul	0.00
76) Pyrene-d10	19.73	212	1572984	32.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1551481	34.13	ng/ul	0.00

Target Compounds						Qvalue
44) Dimethylphthalate	14.07	163	367020	8.82	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG026792.D

Acq On : 1 May 2017 3:28

Operator : SJ/MA

Sample : I2846-15

Misc :

ALS Vial : 29 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

JHSR8


Quant Time: May 01 05:04:03 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon May 01 05:02:38 2017

Response via : Initial Calibration

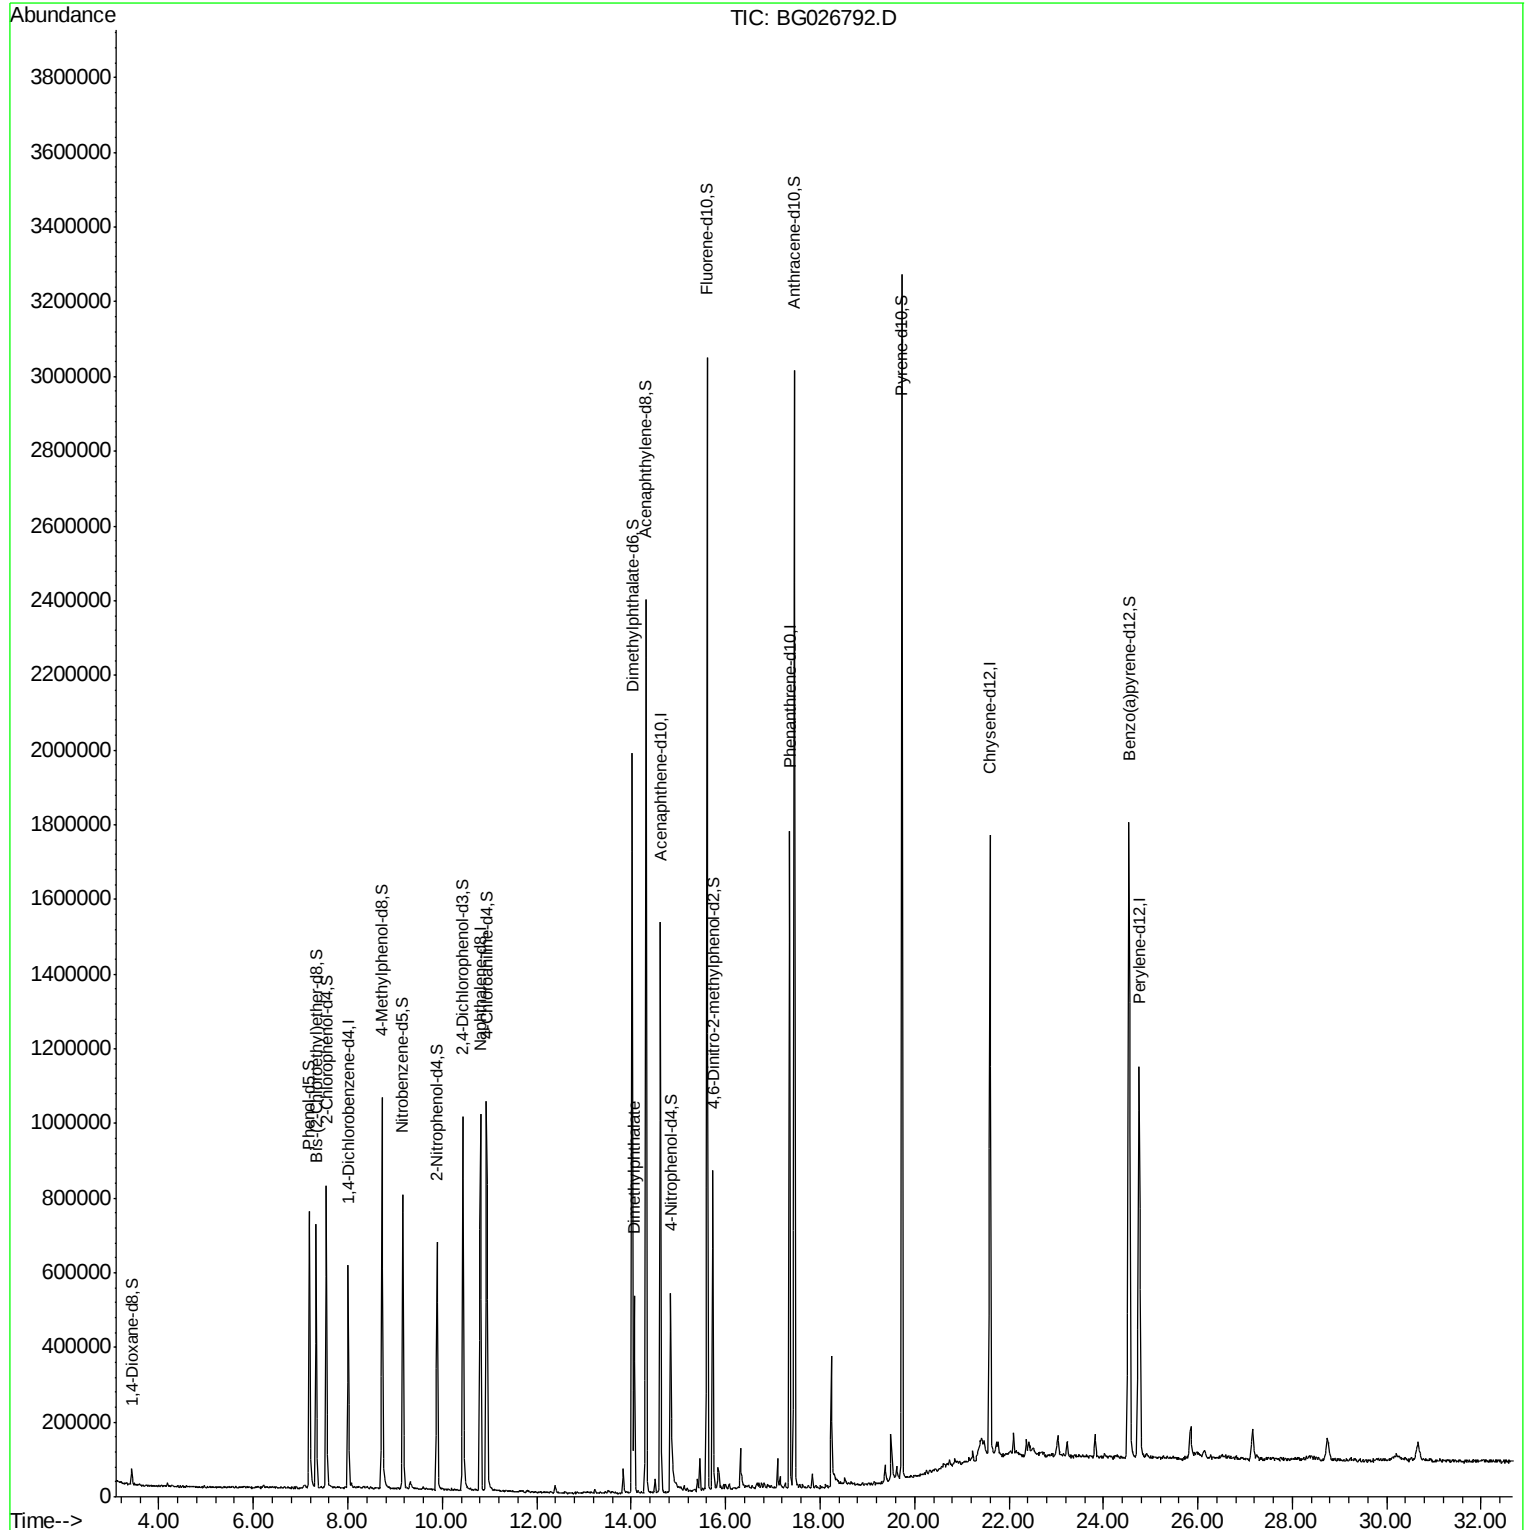

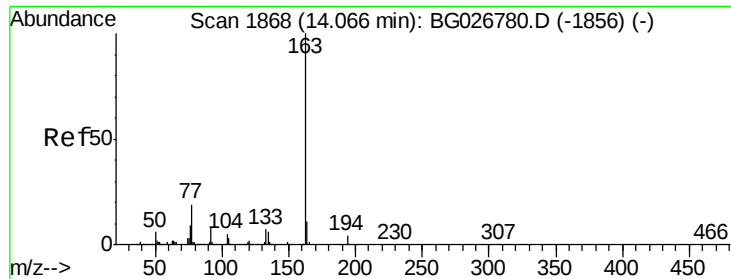

#44

Dimethylphthalate

Concen: 8.82 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. 0.00 min

Lab File: BG026792.D

Acq: 1 May 2017 3:28

Instrument :

BNA_M

ClientSampleId :

JHSR8


Tgt Ion:163 Resp: 367020

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.0

164 10.0 9.0 13.4

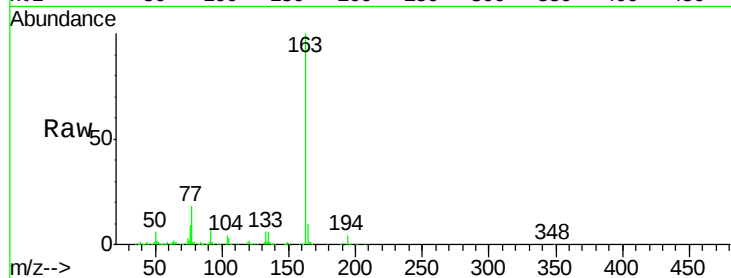

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

