

Data File : BG026794.D
Acq On : 1 May 2017 4:47
Operator : SJ/MA
Sample : I2846-18
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT00

Quant Time: May 01 05:41:31 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 05:02:38 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	182751	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	941509	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	540982	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	1038337	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	950716	20.00	ng/ul	0.00
83) Perylene-d12	24.75	264	977063	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	25261	6.23	ng/uL	0.00
5) Phenol-d5	7.19	99	581638	35.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	945	0.10	ng/ul	0.12
9) 2-Chlorophenol-d4	7.54	132	461414	33.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	499051	36.87	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	255833	32.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	289192	33.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	450366	33.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	722787	39.70	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1428354	32.80	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	1837528	33.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	264416	33.69	ng/ul	0.00
57) Fluorene-d10	15.61	176	1242850	32.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	197406	31.31	ng/ul	0.00
70) Anthracene-d10	17.45	188	1711992	33.97	ng/ul	0.00
76) Pyrene-d10	19.73	212	1623246	32.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1607605	34.80	ng/ul	0.00

Target Compounds						Qvalue
44) Dimethylphthalate	14.07	163	469416	11.01	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG026794.D

Acq On : 1 May 2017 4:47

Operator : SJ/MA

Sample : I2846-18

Misc :

ALS Vial : 31 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

JHT00


Quant Time: May 01 05:41:31 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon May 01 05:02:38 2017

Response via : Initial Calibration

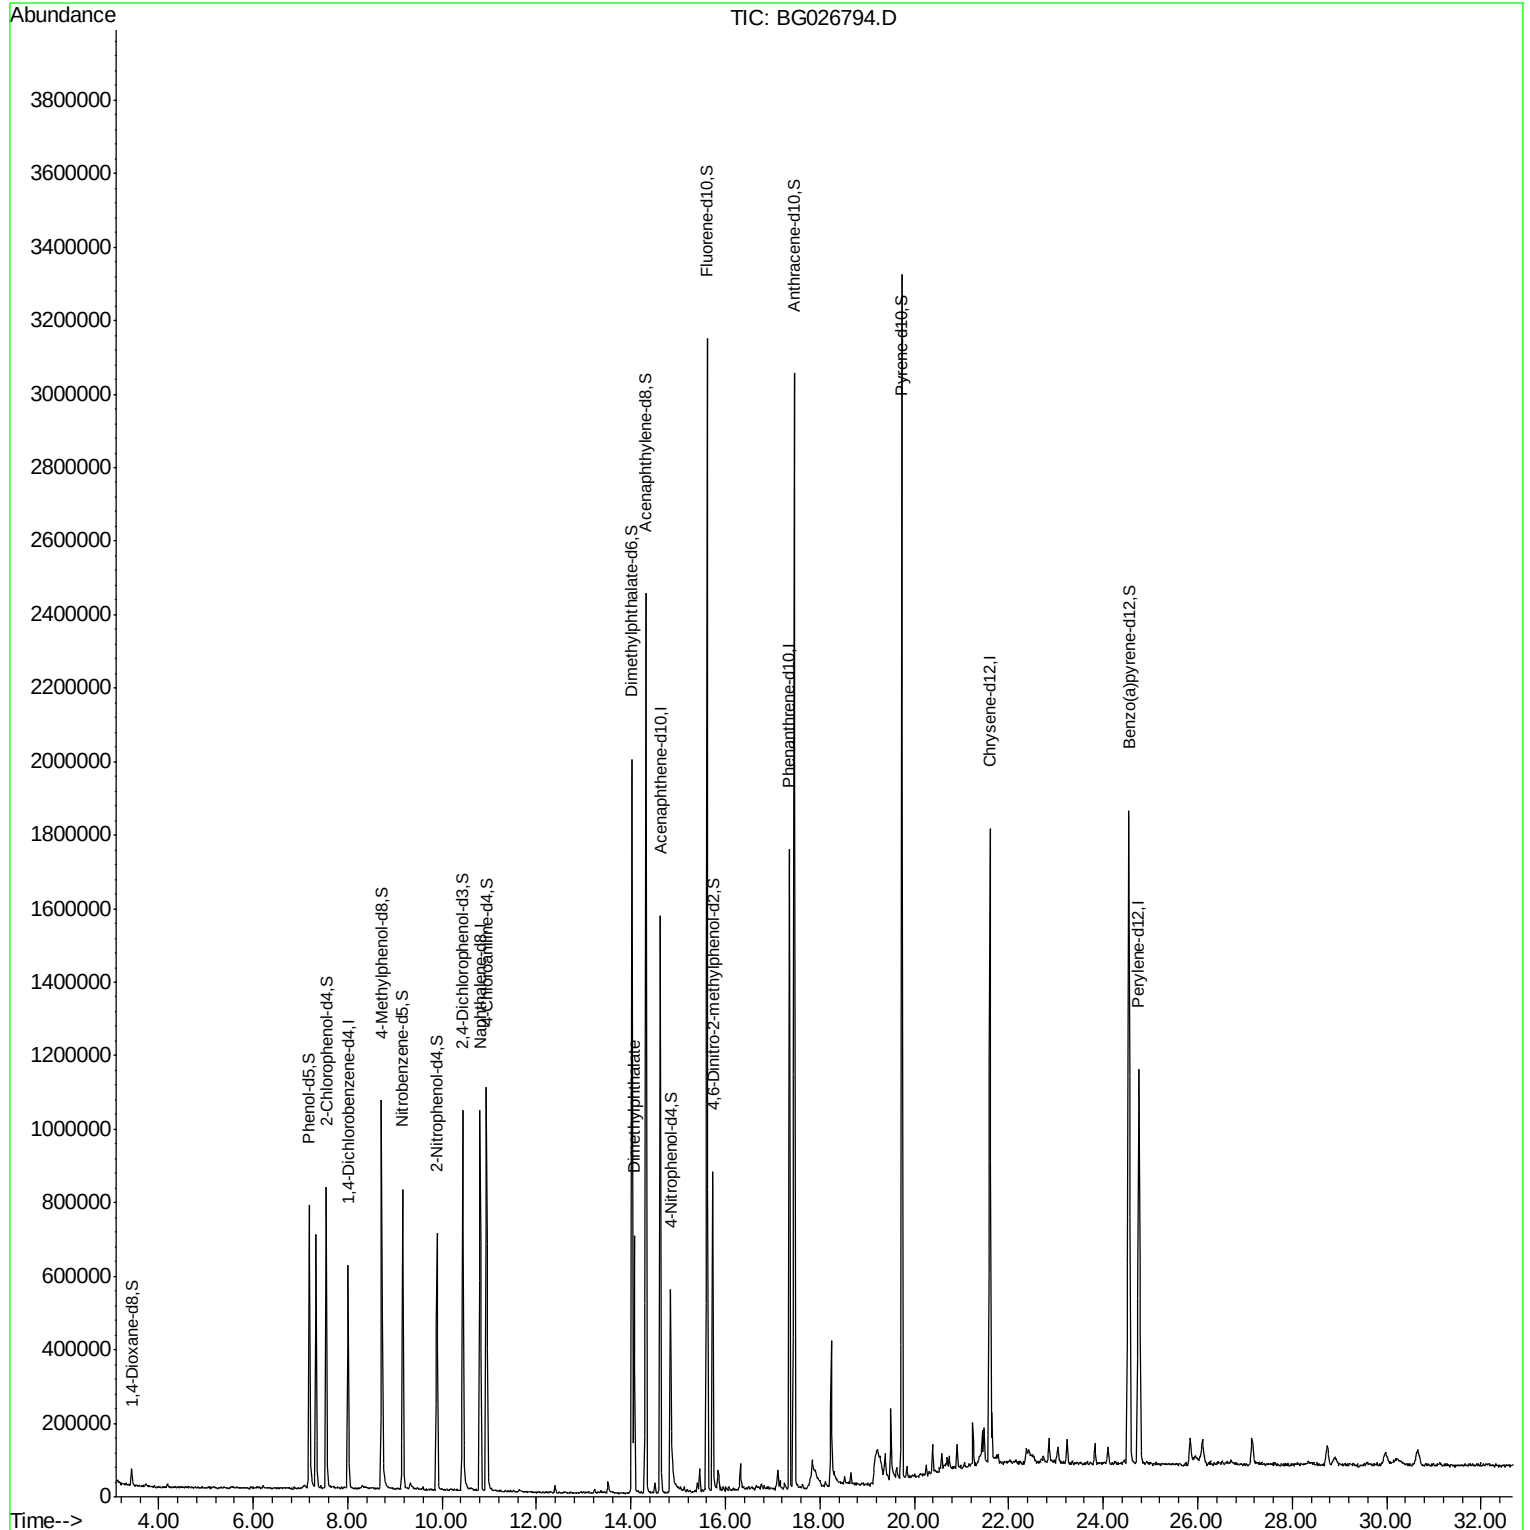

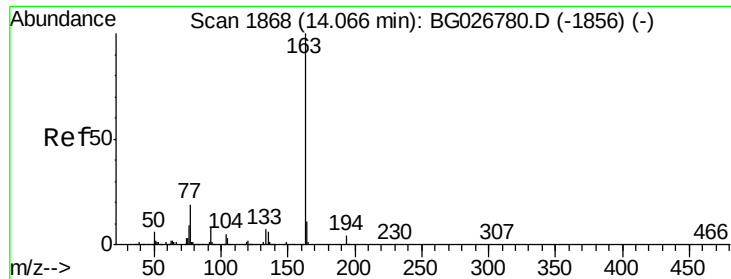

#44

Dimethylphthalate

Concen: 11.01 ng/ul

RT: 14.07 min Scan# 1868

Delta R.T. 0.00 min

Lab File: BG026794.D

Acq: 1 May 2017 4:47

Instrument :

BNA_M

ClientSampleId :

JHT00

Tgt Ion:163 Resp: 469416

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.1 9.0 13.4

