

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043017\
 Data File : BM009827.D
 Acq On : 01 May 2017 00:19
 Operator : SJ/MA
 Sample : I2849-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSX8

Quant Time: May 01 02:30:49 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 01 02:28:42 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	209400	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	859315	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	526684	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1198987	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	966509	20.00	ng/ul	0.00
83) Perylene-d12	23.72	264	901422	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	16983	3.73	ng/uL	0.00
5) Phenol-d5	6.99	99	386174	16.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	265725	17.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	266536	18.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	284769	16.06	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	136769	19.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	153568	20.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	279349	18.98	ng/ul	0.01
29) 4-Chloroaniline-d4	10.76	131	274495	15.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	888636	19.40	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1137195	20.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	124792	14.12	ng/ul	0.01
57) Fluorene-d10	15.46	176	836156	20.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	63433	7.50	ng/ul	0.00
70) Anthracene-d10	17.32	188	1284953	20.87	ng/ul	0.00
76) Pyrene-d10	19.61	212	1165548	27.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	922039	21.03	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.92	163	163820	3.61	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043017\
Data File : BM009827.D
Acq On : 01 May 2017 00:19
Operator : SJ/MA
Sample : I2849-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSX8

Quant Time: May 01 02:30:49 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 01 02:28:42 2017
Response via : Initial Calibration

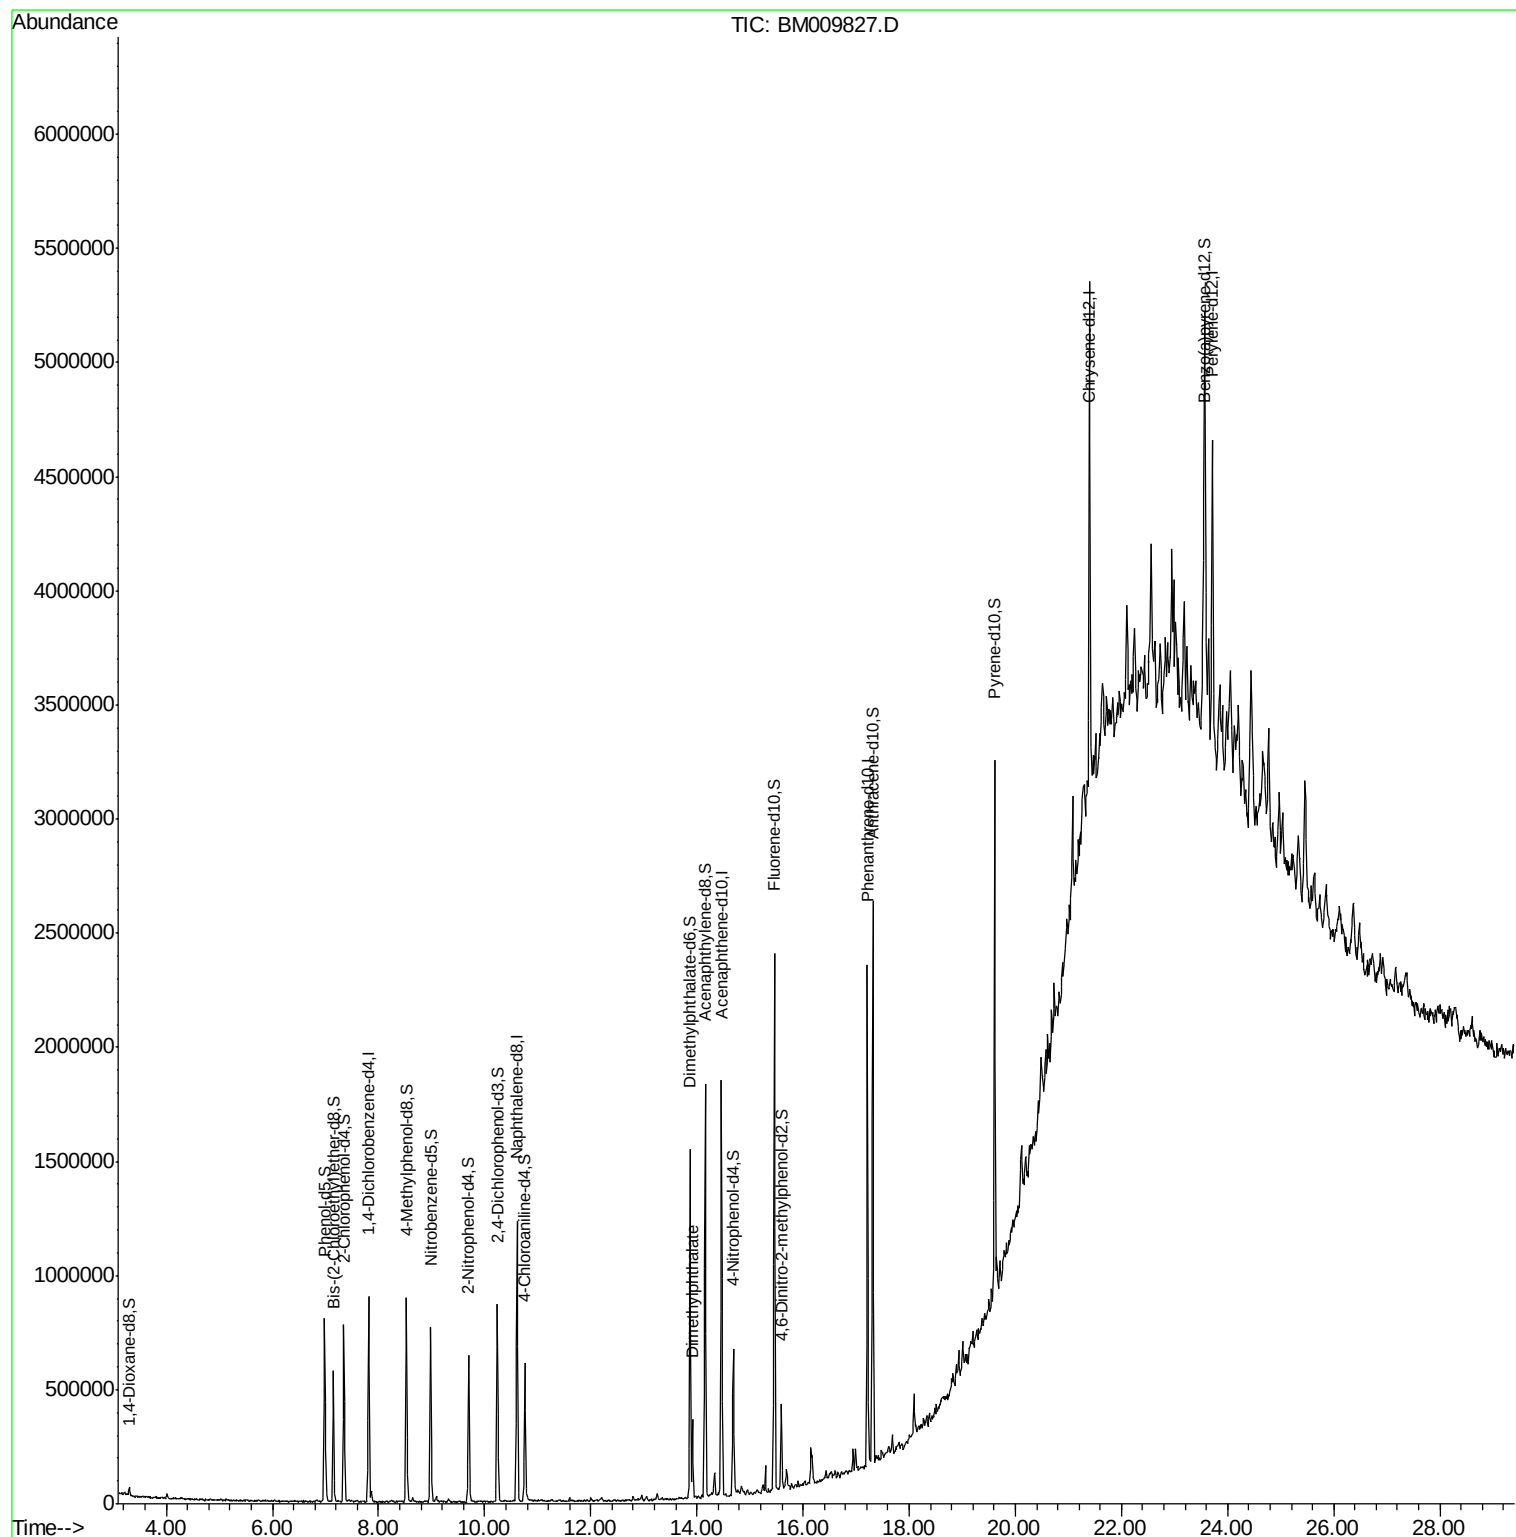


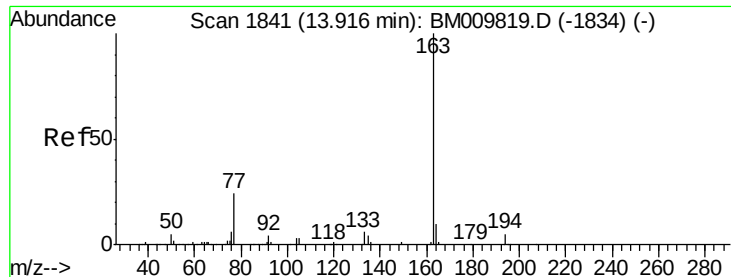

#44
 Dimethylphthalate
 Concen: 3.61 ng/ul
 RT: 13.92 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: BM009827.D
 Acq: 01 May 2017 00:19

Instrument :
 BNA_M
 ClientSampleId :
 JHSX8

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.0	4.6
164	10.8	8.6	12.8

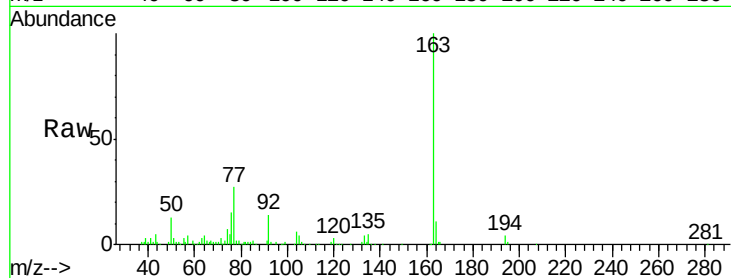

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

