

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
 Data File : BM014861.D
 Acq On : 30 Apr 2018 11:37
 Operator : SJ/JU
 Sample : J2603-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 01 03:06:14 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 01 03:05:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	423340	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1792663	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	942107	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1954061	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1712752	20.00	ng/ul	0.00
83) Perylene-d12	24.39	264	1603299	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.64	96	56571	5.83	ng/uL	0.00
5) Phenol-d5	7.62	99	110119	3.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	350878	16.72	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	345921	12.64	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	193278	7.41	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	190332	14.68	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	195039	15.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	344354	13.13	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	2206	0.09	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	1132727	15.40	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	1264851	13.93	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	24571	1.80	ng/ul	0.00
57) Fluorene-d10	16.08	176	964427	15.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	112636	10.65	ng/ul	0.00
70) Anthracene-d10	17.92	188	1403685	15.41	ng/ul	0.00
76) Pyrene-d10	20.15	212	1425395	17.59	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.23	264	1291938	16.40	ng/ul	0.00
Target Compounds						
6) Phenol	7.65	94	124830	3.877	ng/ul#	82
44) Dimethylphthalate	14.54	163	475373	6.687	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
Data File : BM014861.D
Acq On : 30 Apr 2018 11:37
Operator : SJ/JU
Sample : J2603-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 01 03:06:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 03:05:17 2018
Response via : Initial Calibration

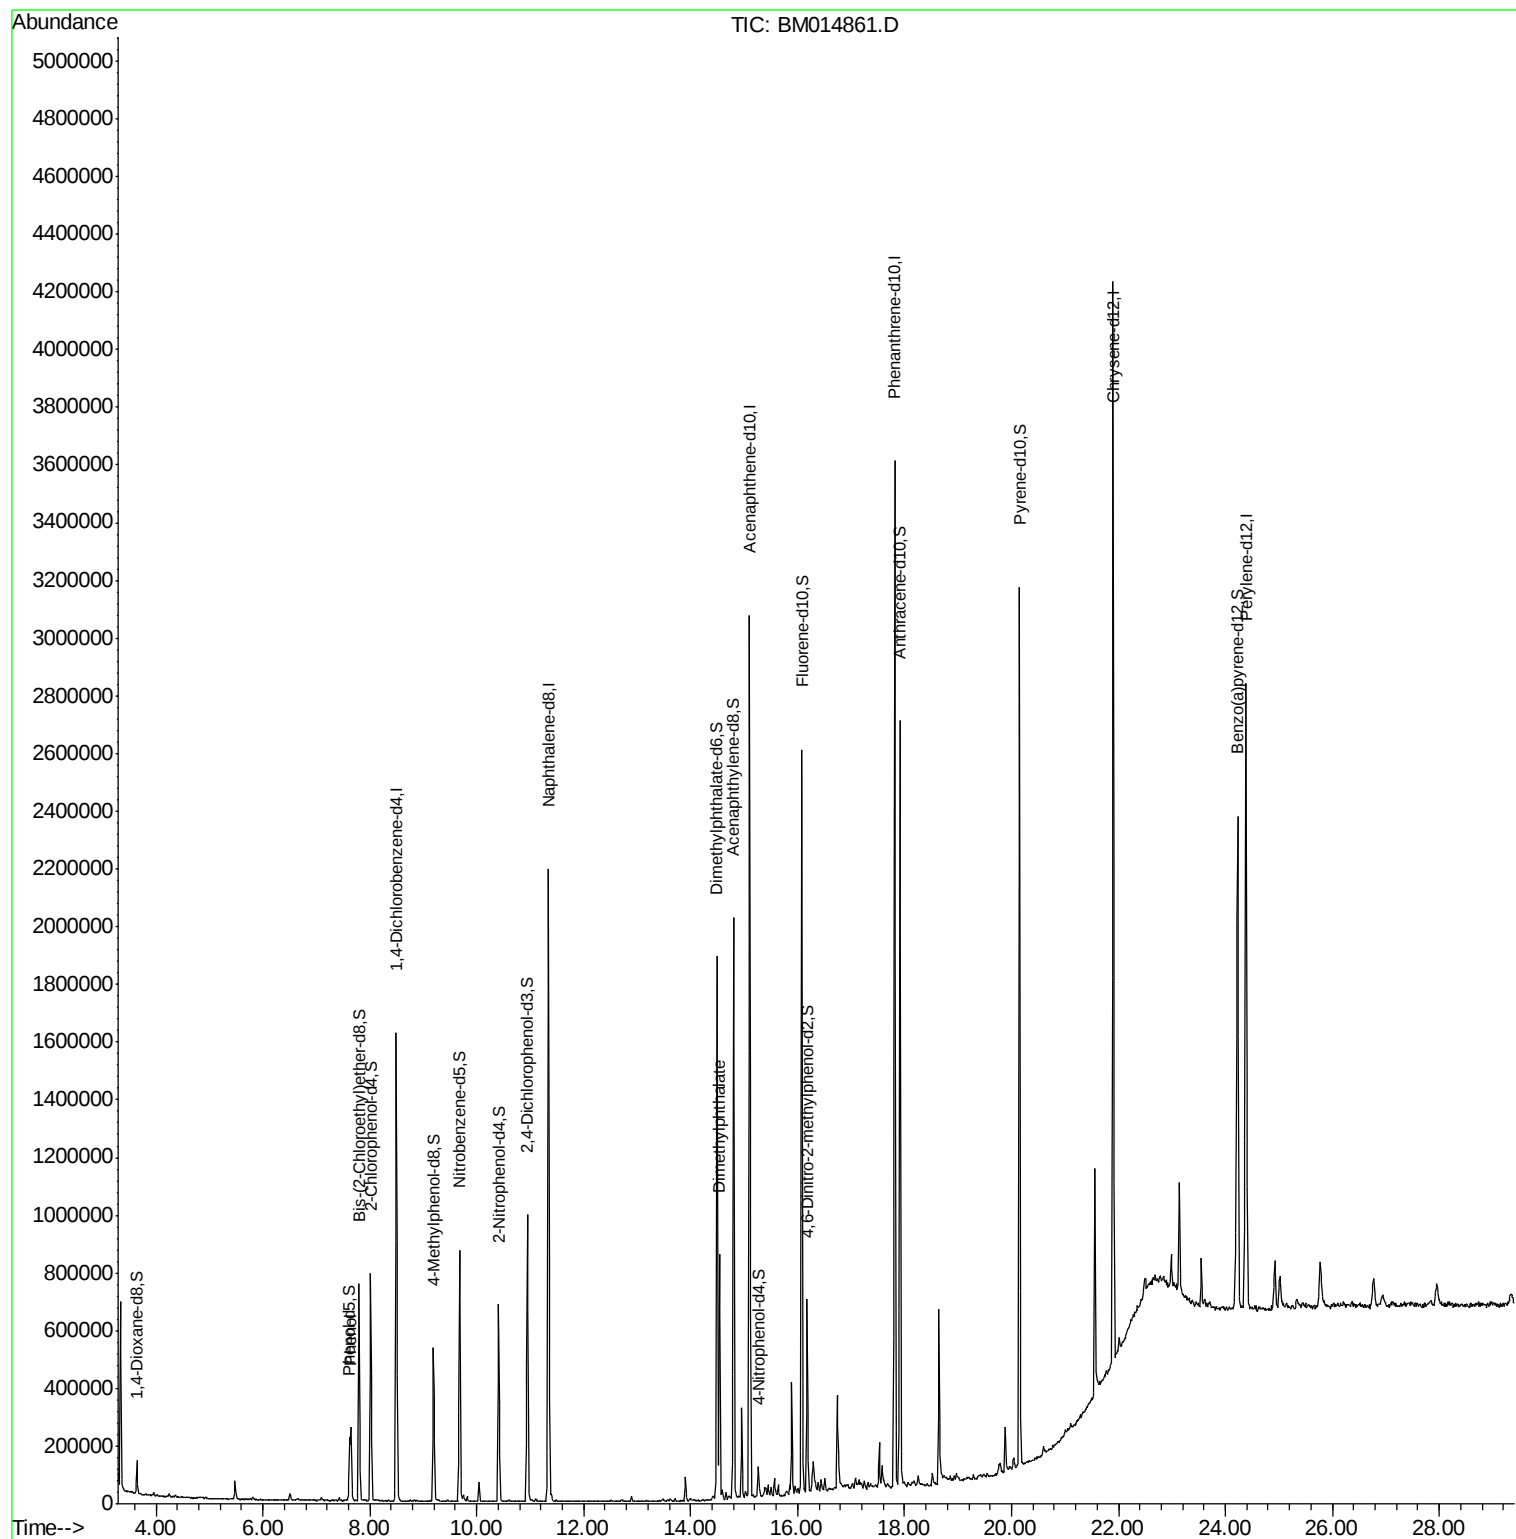

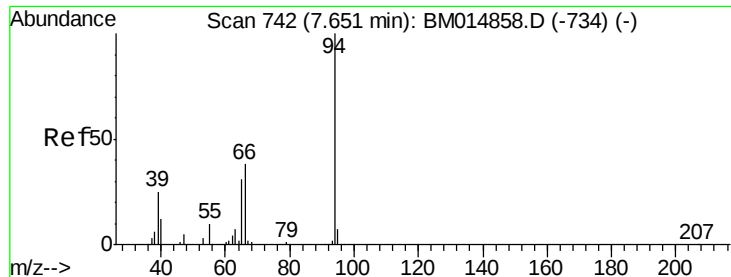

#6

Phenol

Concen: 3.877 ng/ul

RT: 7.65 min Scan# 741

Delta R.T. -0.01 min

Lab File: BM014861.D

Acq: 30 Apr 2018 11:37

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 124830

Ion Ratio Lower Upper

94 100

65 31.7 28.2 42.4




66 40.1 47.2 70.8#

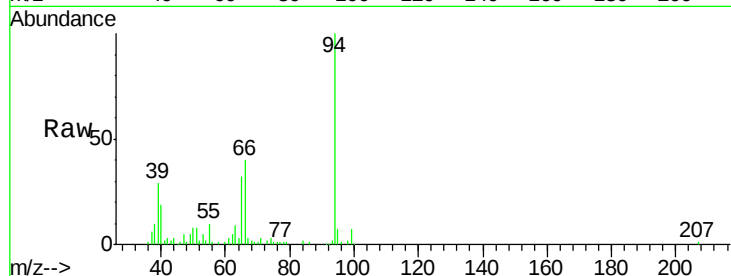

Abundance Ion 94.00 (93.70 to 94.70): BM014858.D (-734) (-)

Ion 65.00 (64.70 to 65.70): BM014858.D (-734) (-)

Ion 66.00 (65.70 to 66.70): BM014858.D (-734) (-)

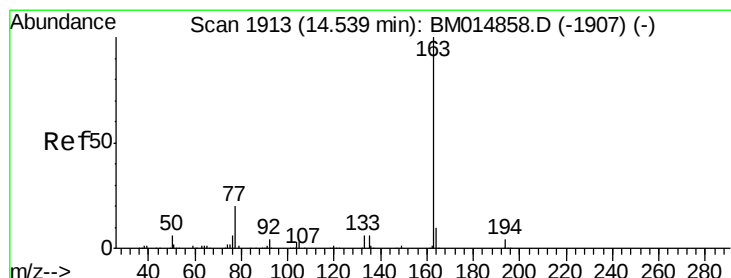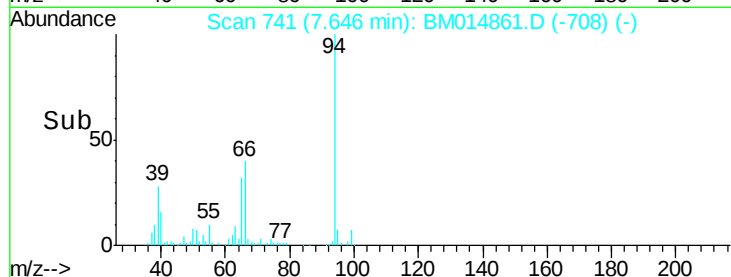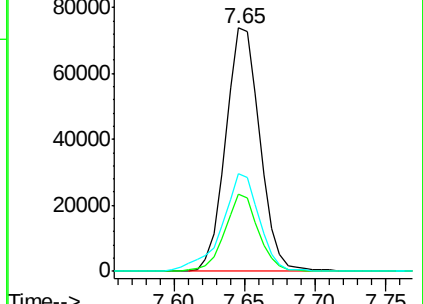

#44

Dimethylphthalate

Concen: 6.687 ng/ul

RT: 14.54 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BM014861.D

Acq: 30 Apr 2018 11:37


Tgt Ion:163 Resp: 475373

Ion Ratio Lower Upper

163 100

194 3.9 3.5 5.3

164 9.6 8.2 12.4

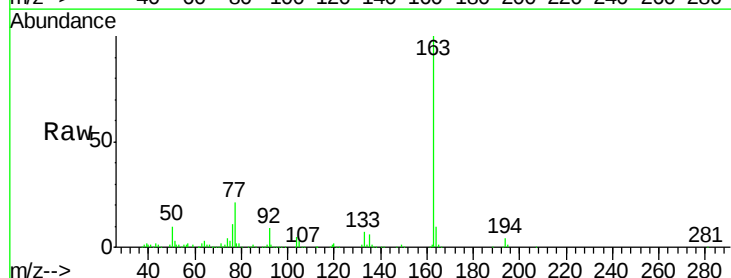

Abundance Ion 163.00 (162.70 to 163.70): BM014858.D (-1907) (-)

Ion 194.00 (193.70 to 194.70): BM014858.D (-1907) (-)

Ion 164.00 (163.70 to 164.70): BM014858.D (-1907) (-)

