

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
 Data File : BM014869.D
 Acq On : 30 Apr 2018 16:27
 Operator : SJ/JU
 Sample : J2603-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 01 03:07:52 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 01 03:05:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	342587	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1396793	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	680440	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1452671	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1412337	20.00	ng/ul	0.00
83) Perylene-d12	24.39	264	1206613	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.64	96	51350	6.54	ng/uL	0.00
5) Phenol-d5	7.62	99	138281	5.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	401201	23.62	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	410320	18.52	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	240505	11.39	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	221561	21.94	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	218725	21.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	376239	18.41	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	398	0.02	ng/ul	0.01
43) Dimethylphthalate-d6	14.49	166	1262290	23.77	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	1165733	17.77	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	33261	3.37	ng/ul	0.00
57) Fluorene-d10	16.08	176	1055439	22.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	133046	16.93	ng/ul	0.00
70) Anthracene-d10	17.92	188	1480467	21.87	ng/ul	0.00
76) Pyrene-d10	20.15	212	1544450	23.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.23	264	1249368	21.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.54	163	58277	1.135	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
Data File : BM014869.D
Acq On : 30 Apr 2018 16:27
Operator : SJ/JU
Sample : J2603-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 01 03:07:52 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 03:05:17 2018
Response via : Initial Calibration

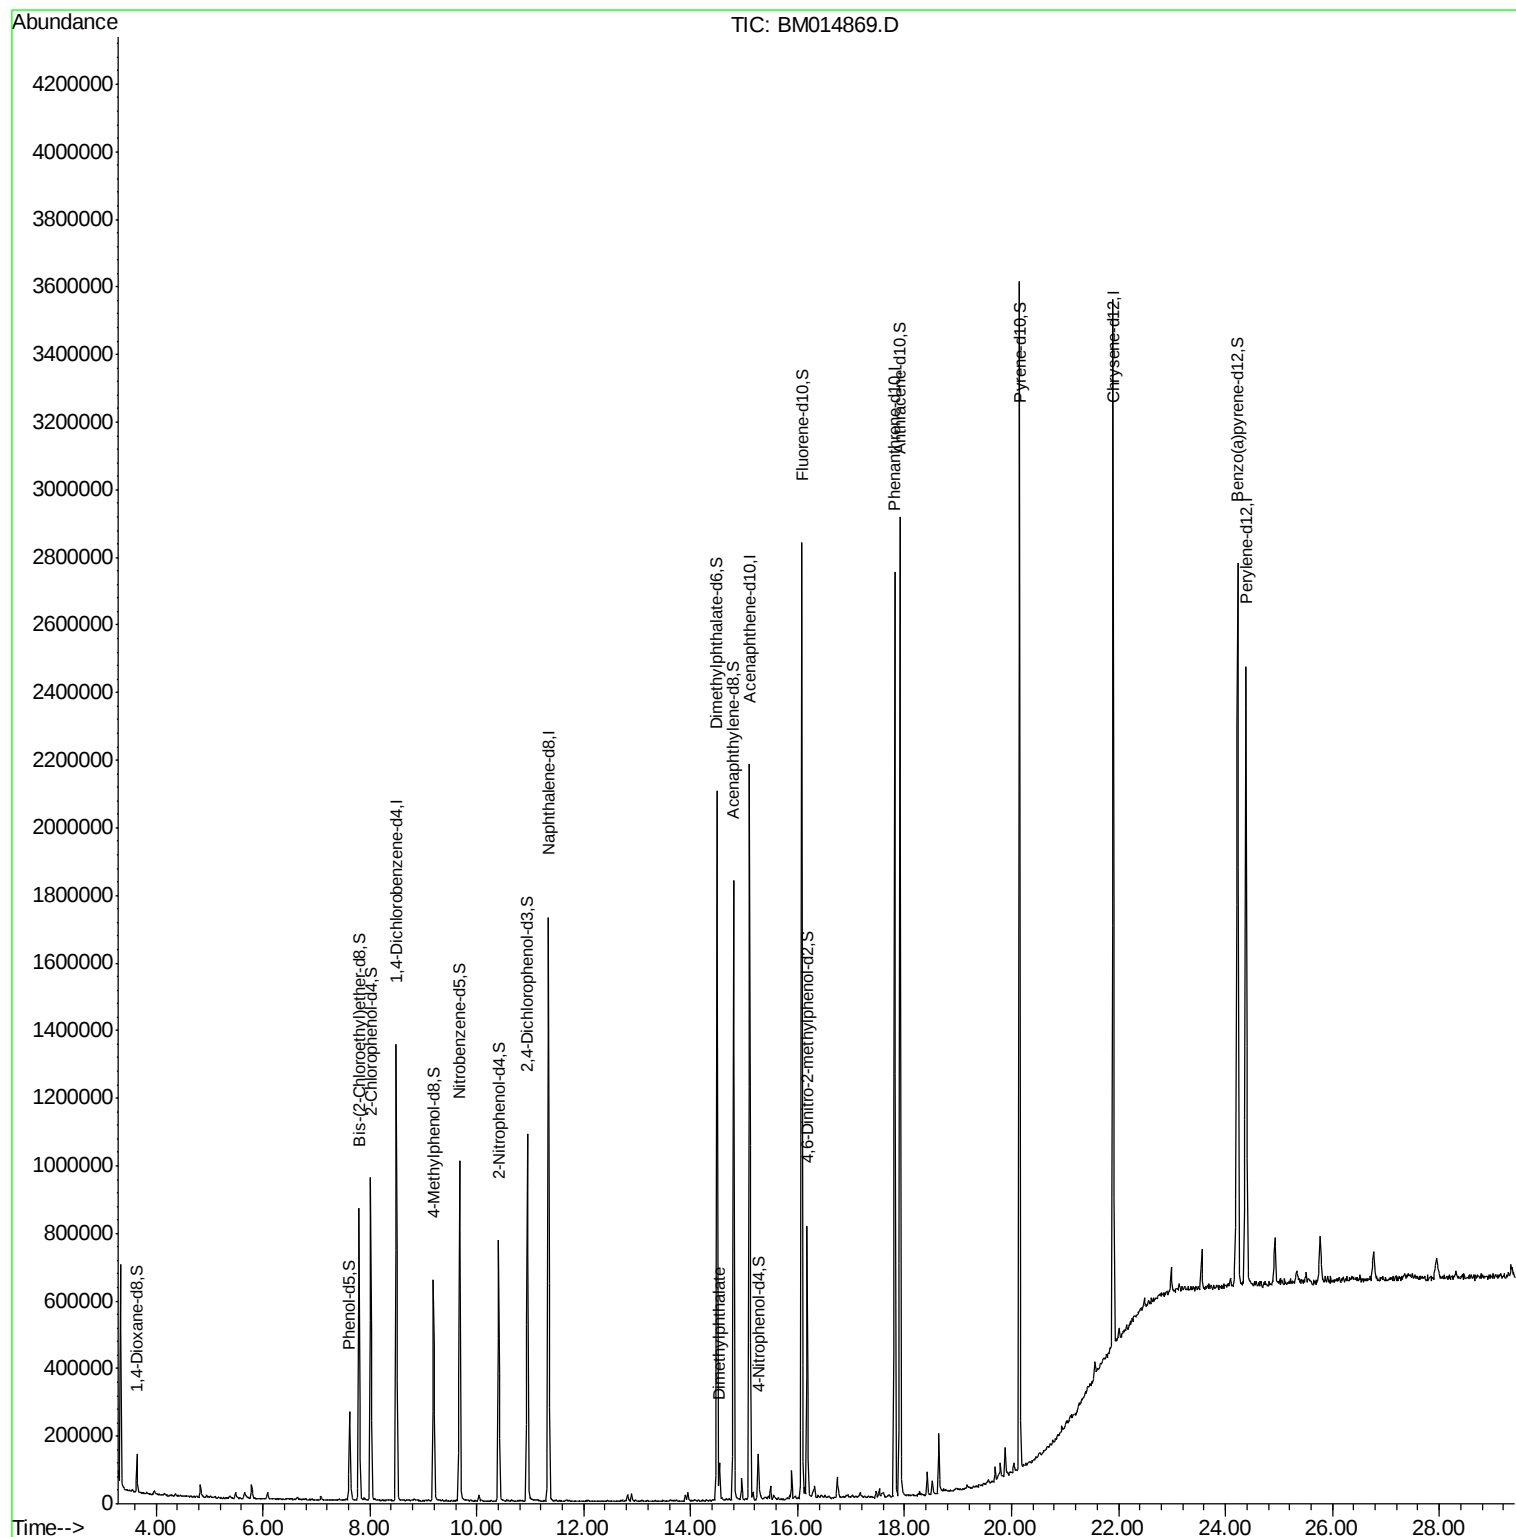


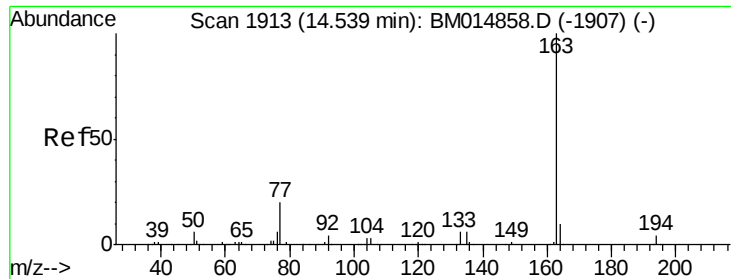

#44
 Dimethylphthalate
 Concen: 1.135 ng/ul
 RT: 14.54 min Scan# 1913
 Delta R.T. -0.00 min
 Lab File: BM014869.D
 Acq: 30 Apr 2018 16:27

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:163 Resp: 58277
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.5 5.3
 164 10.7 8.2 12.4

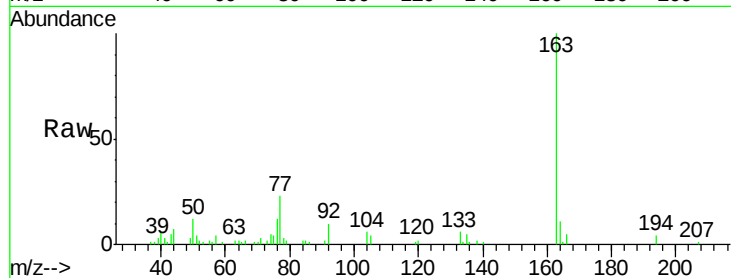

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

