

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
 Data File : BM014872.D
 Acq On : 30 Apr 2018 18:17
 Operator : SJ/JU
 Sample : J2603-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F1B59

Quant Time: May 01 03:41:58 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 01 03:41:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	396803	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1616855	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	805490	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1651944	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1589934	20.00	ng/ul	0.00
83) Perylene-d12	24.39	264	1644467	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	56675	6.24	ng/uL	0.00
5) Phenol-d5	7.62	99	82955	2.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	256416	13.04	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	253443	9.88	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	144505	5.91	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	136717	11.70	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	132775	11.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	239675	10.13	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	7781	0.33	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	776107	12.34	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	890332	11.47	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	16443	1.41	ng/ul	0.00
57) Fluorene-d10	16.08	176	669609	12.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	70583	7.90	ng/ul	0.00
70) Anthracene-d10	17.91	188	963066	12.51	ng/ul	0.00
76) Pyrene-d10	20.15	212	982720	13.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	1071326	13.26	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	7.65	94	59103	1.958	ng/ul# 81
44) Dimethylphthalate	14.54	163	270130	4.444	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
Data File : BM014872.D
Acq On : 30 Apr 2018 18:17
Operator : SJ/JU
Sample : J2603-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F1B59

Quant Time: May 01 03:41:58 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 03:41:22 2018
Response via : Initial Calibration

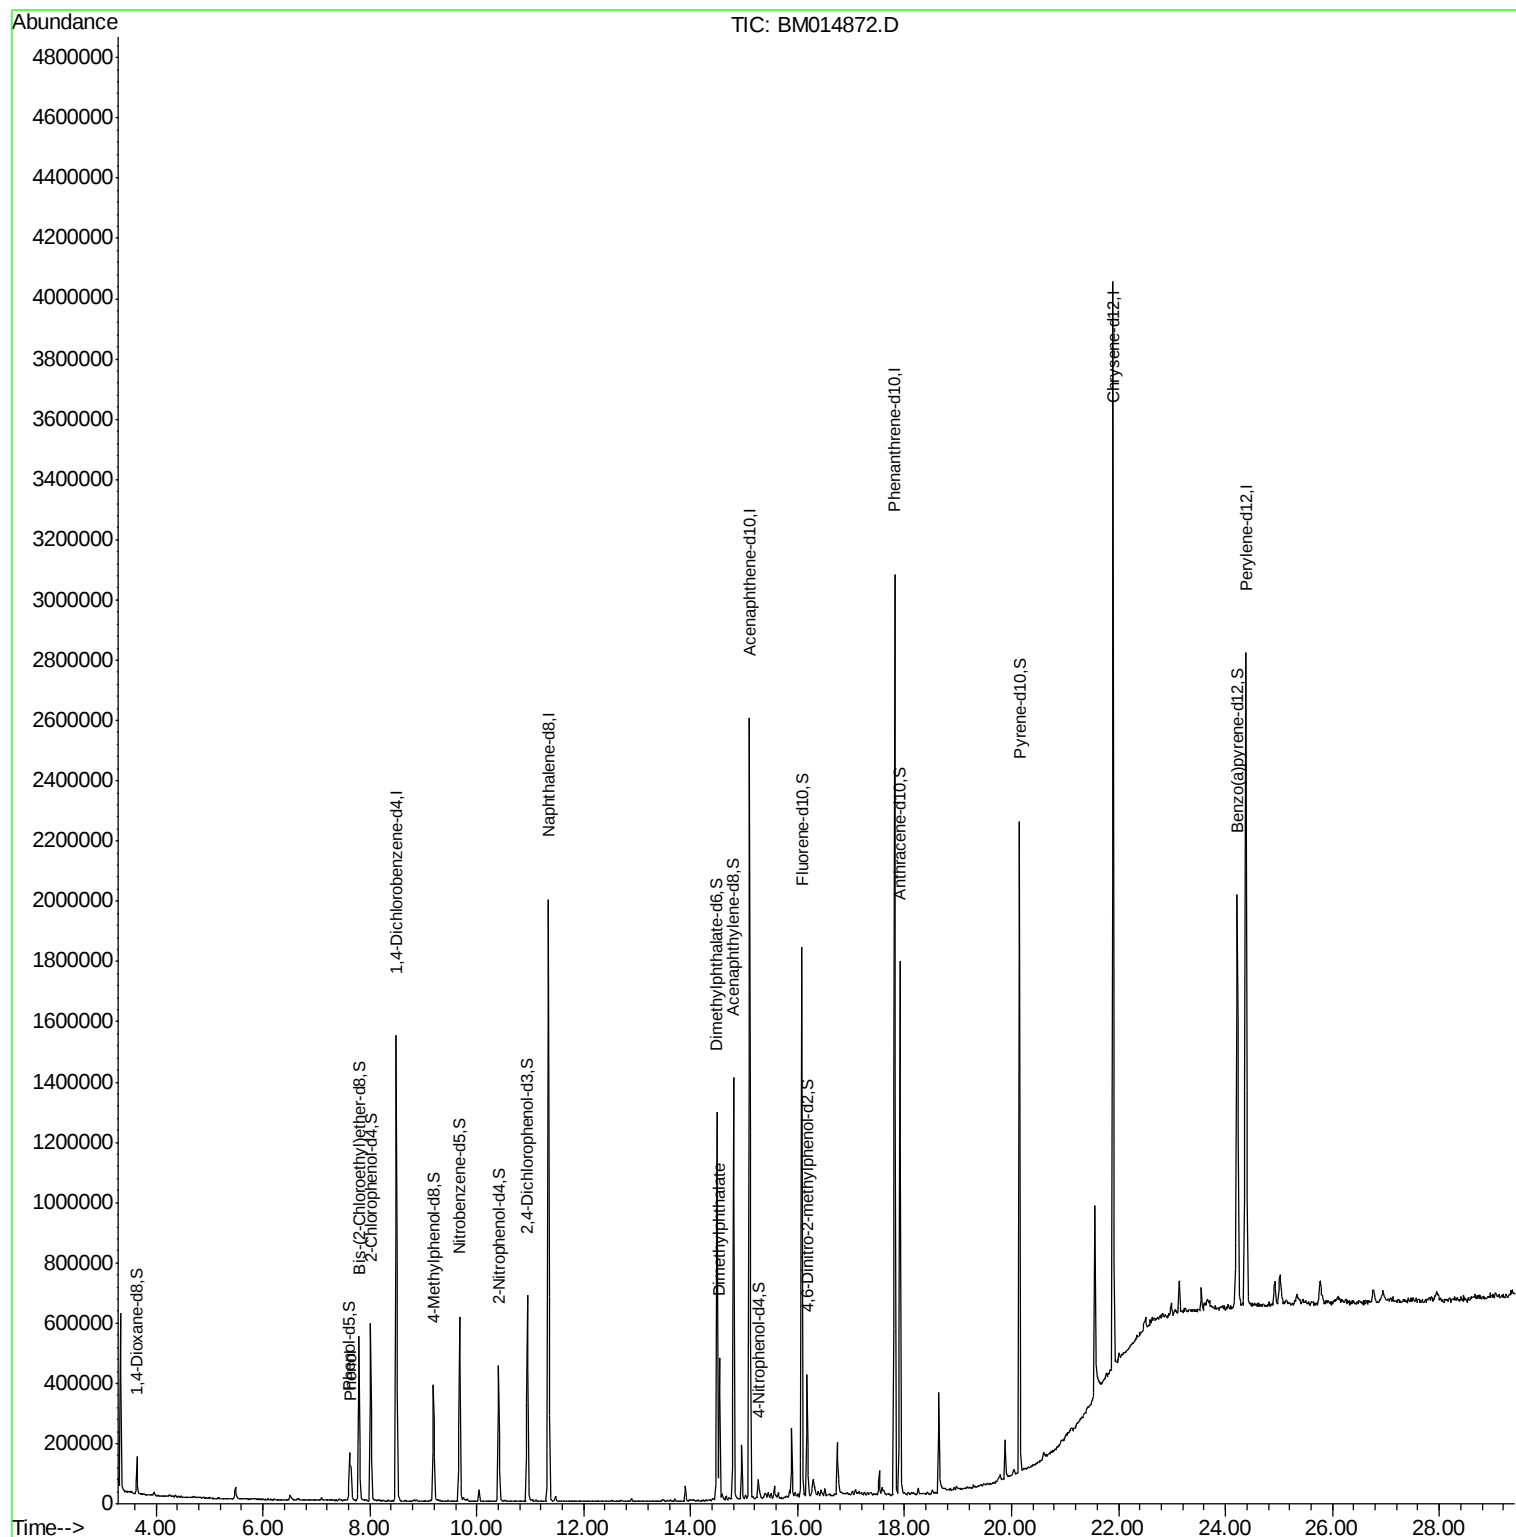

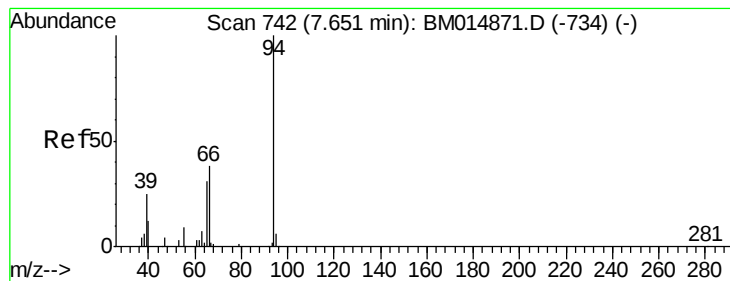





#6

Phenol

Concen: 1.958 ng/ul
 RT: 7.65 min Scan# 741
 Delta R.T. -0.01 min
 Lab File: BM014872.D
 Acq: 30 Apr 2018 18:17

Instrument :
 BNA_M
 ClientSampleId :
 F1B59

Tot Ion	Ratio	Lower	Upper
94	100		
65	31.9	28.2	42.4
66	38.8	47.2	70.8#

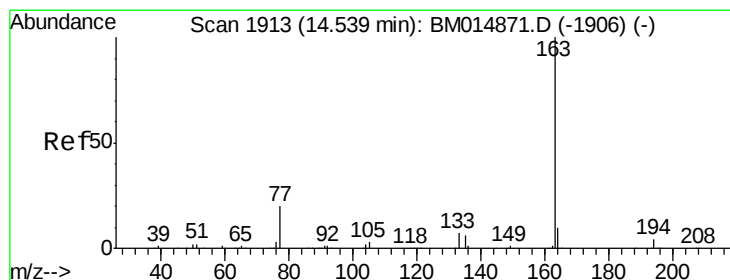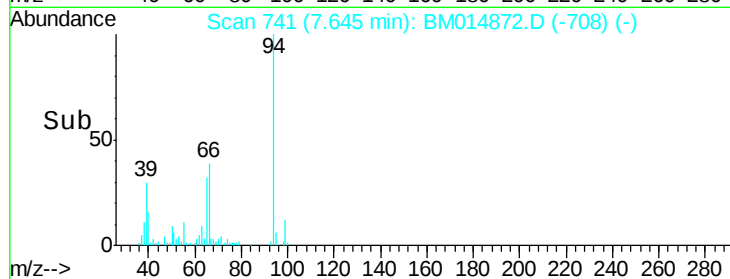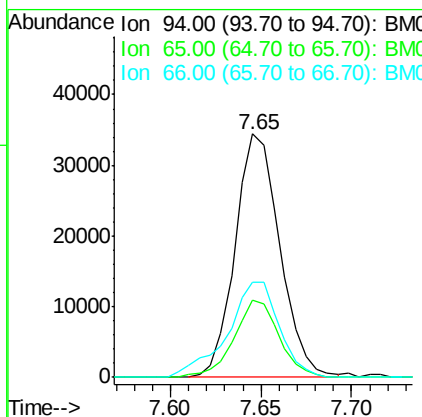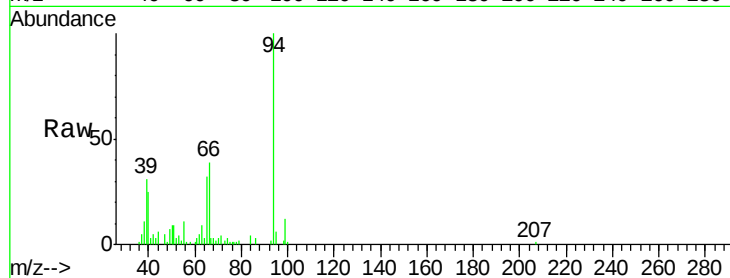

#44

Dimethylphthalate

Concen: 4.444 ng/ul
 RT: 14.54 min Scan# 1913
 Delta R.T. 0.00 min
 Lab File: BM014872.D
 Acq: 30 Apr 2018 18:17

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.5	5.3
164	10.3	8.2	12.4

