

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
 Data File : BM014879.D
 Acq On : 30 Apr 2018 22:32
 Operator : SJ/JU
 Sample : J2551-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F1B57

Quant Time: May 01 03:43:29 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 01 03:41:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	354994	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1501718	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	790482	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1696301	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1776157	20.00	ng/ul	0.00
83) Perylene-d12	24.39	264	1761118	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.65	96	57505	7.07	ng/uL	0.00
5) Phenol-d5	7.62	99	217125	7.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	620248	35.24	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	626525	27.29	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	388280	17.74	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	354619	32.66	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	368090	34.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	634649	28.89	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	51170	2.36	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	2085028	33.79	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2422216	31.79	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	64301	5.61	ng/ul	0.00
57) Fluorene-d10	16.08	176	1755151	32.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	252127	27.47	ng/ul	0.00
70) Anthracene-d10	17.92	188	2665658	33.72	ng/ul	0.00
76) Pyrene-d10	20.15	212	2866642	34.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	3114886	36.00	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	7.65	94	27367	1.014	ng/ul#	85
44) Dimethylphthalate	14.54	163	175848	2.948	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
Data File : BM014879.D
Acq On : 30 Apr 2018 22:32
Operator : SJ/JU
Sample : J2551-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F1B57

Quant Time: May 01 03:43:29 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 03:41:22 2018
Response via : Initial Calibration

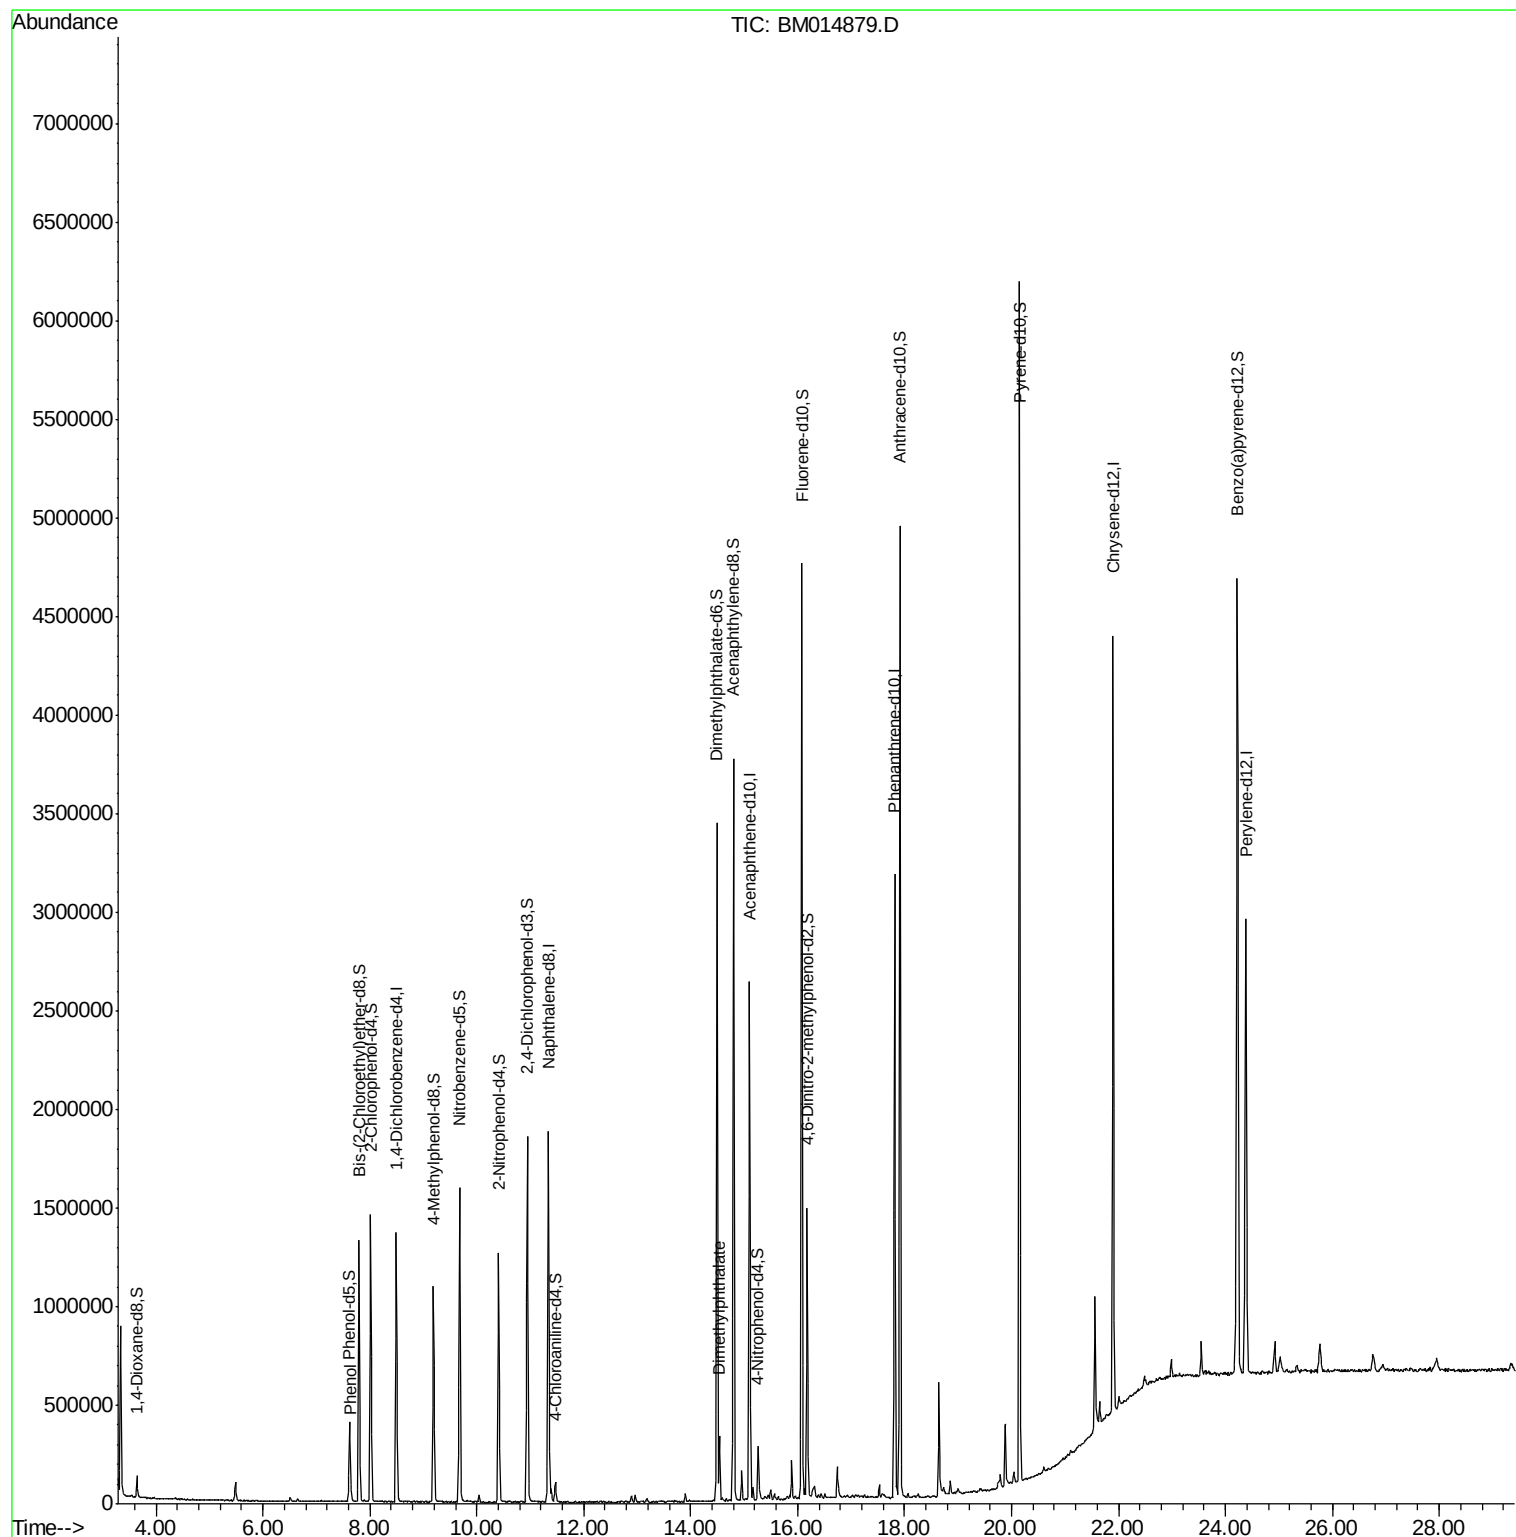

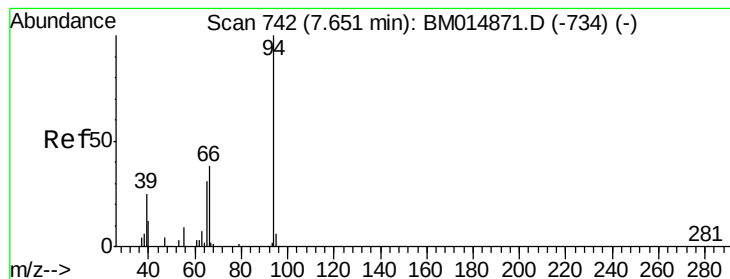





#6

Phenol

Concen: 1.014 ng/ul
 RT: 7.65 min Scan# 741
 Delta R.T. -0.01 min
 Lab File: BM014879.D
 Acq: 30 Apr 2018 22:32

Instrument :
 BNA_M
 ClientSampleId :
 F1B57

Tot Ion: 94 Resp: 27367
 Ion Ratio Lower Upper
 94 100
 65 31.6 28.2 42.4
 66 44.3 47.2 70.8#

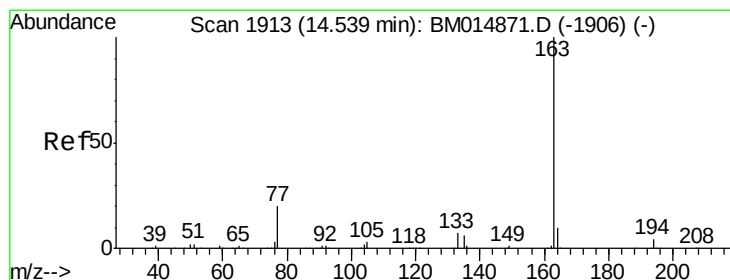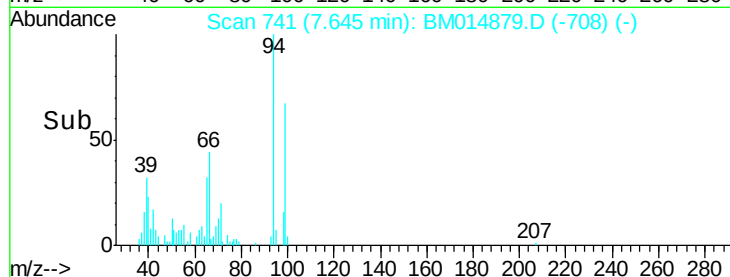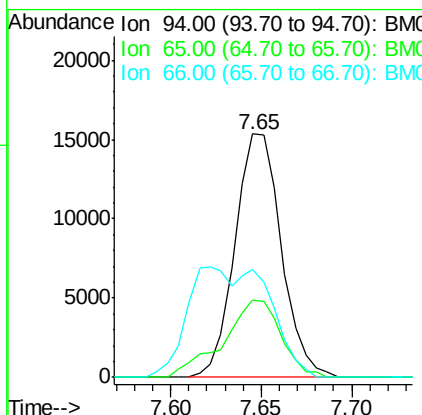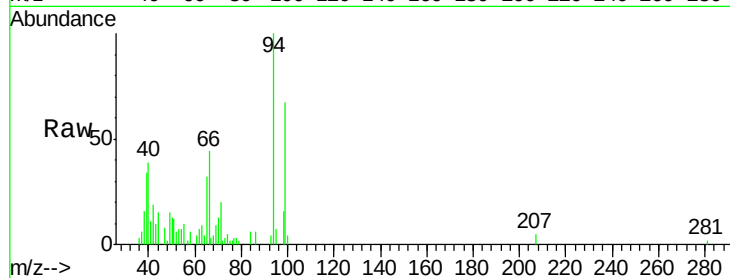

#44

Dimethylphthalate

Concen: 2.948 ng/ul
 RT: 14.54 min Scan# 1913
 Delta R.T. 0.00 min
 Lab File: BM014879.D
 Acq: 30 Apr 2018 22:32

Tgt Ion: 163 Resp: 175848
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.5 5.3
 164 10.0 8.2 12.4

