

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
 Data File : BM014884.D
 Acq On : 01 May 2018 01:33
 Operator : SJ/JU
 Sample : J2603-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F1B67

Quant Time: May 01 03:44:46 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 01 03:41:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	452300	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1884268	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	956223	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1912130	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1615647	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1563503	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.65	96	24864	2.40	ng/uL	0.00
5) Phenol-d5	7.62	99	443435	12.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	315699	14.08	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	376058	12.86	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	352818	12.65	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	165865	12.17	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	162576	11.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	317792	11.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	466112	17.13	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	959375	12.85	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	1084071	11.76	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	82907	5.98	ng/ul	0.00
57) Fluorene-d10	16.07	176	801985	12.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	56995	5.51	ng/ul	0.00
70) Anthracene-d10	17.91	188	1183978	13.29	ng/ul	0.00
76) Pyrene-d10	20.15	212	1171521	15.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	1099921	14.32	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.54	163	187077	2.593	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
Data File : BM014884.D
Acq On : 01 May 2018 01:33
Operator : SJ/JU
Sample : J2603-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F1B67

Quant Time: May 01 03:44:46 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 03:41:22 2018
Response via : Initial Calibration

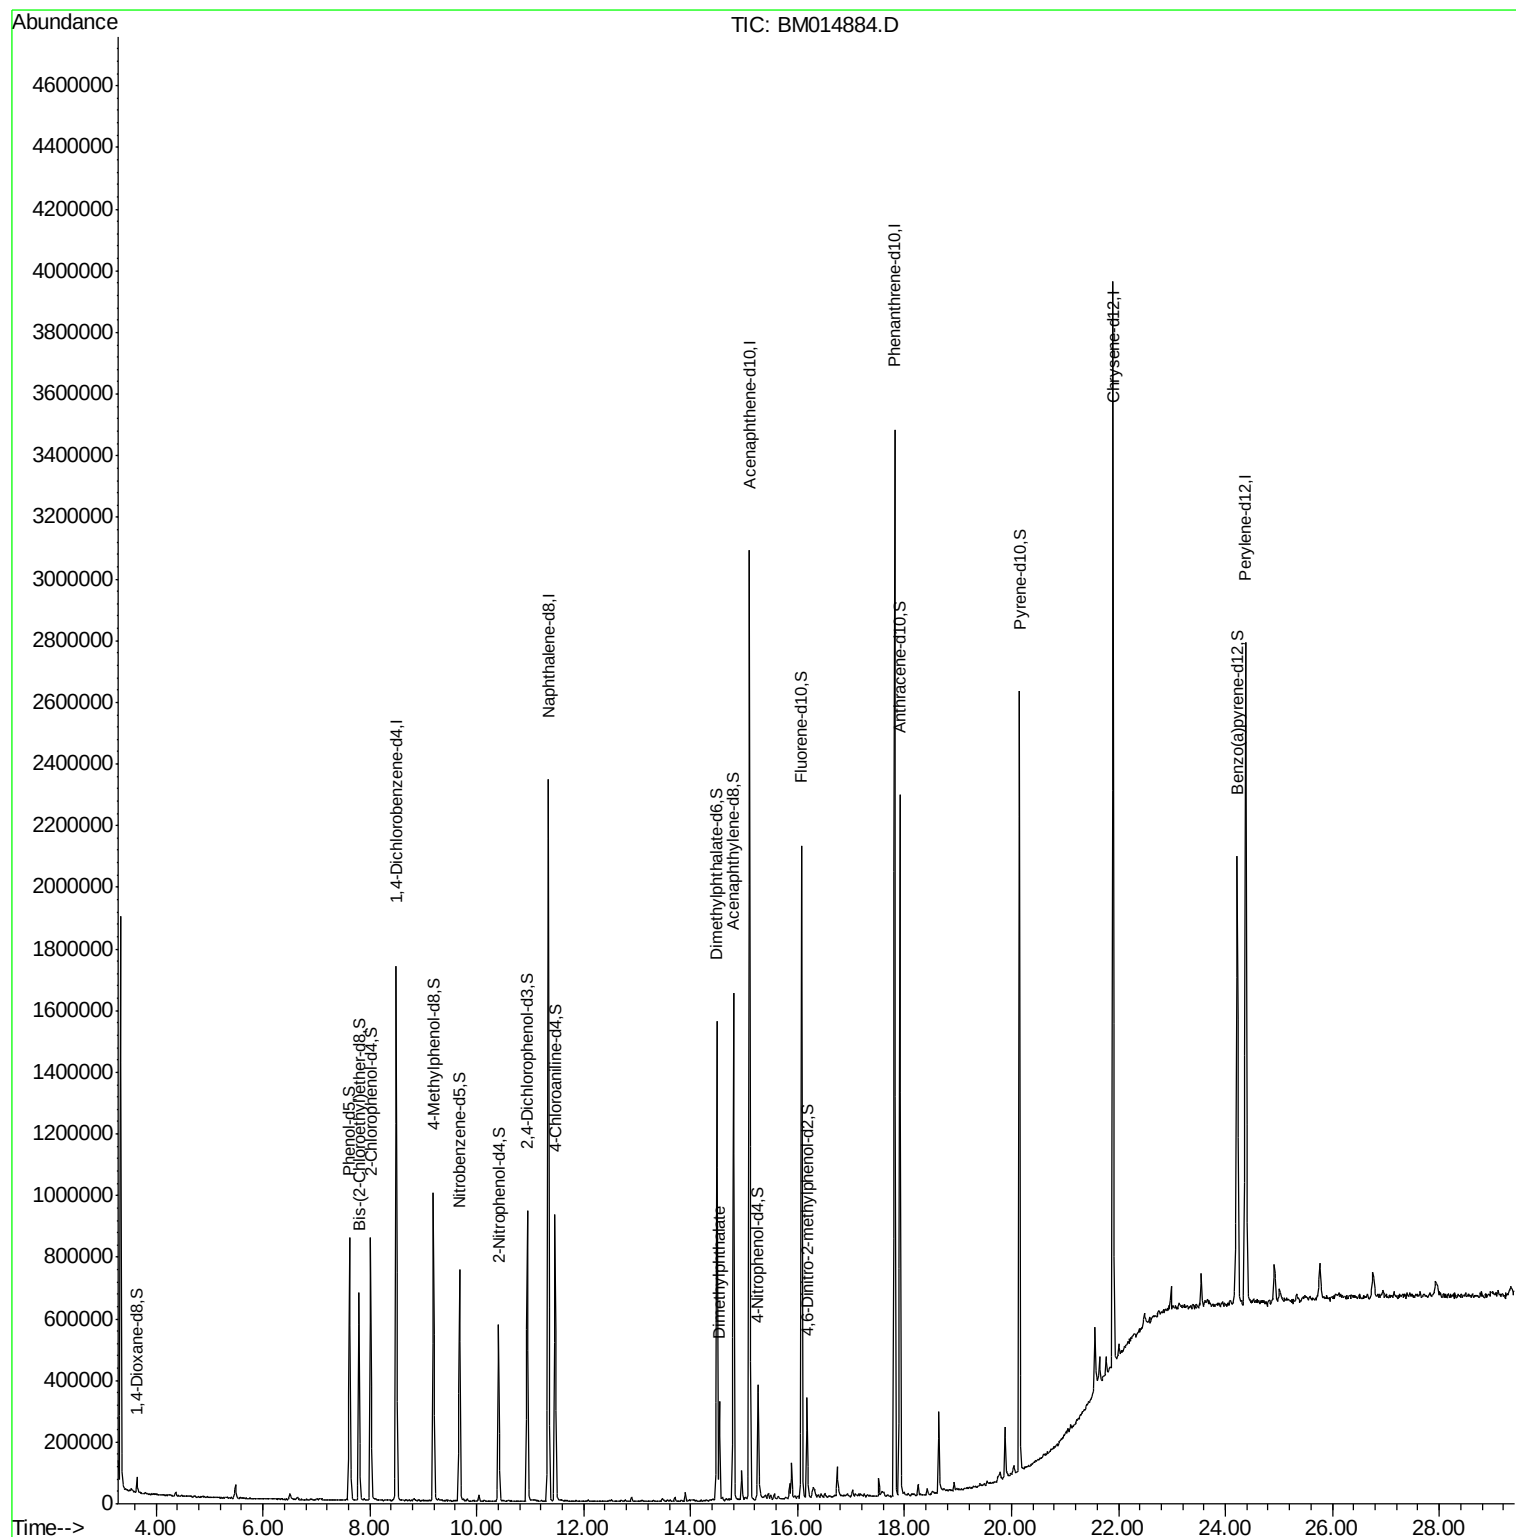

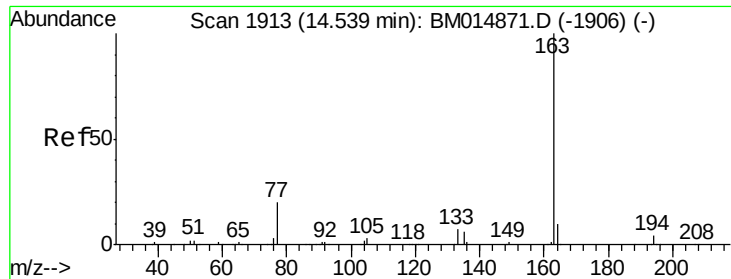

#44

Dimethylphthalate

Concen: 2.593 ng/ul

RT: 14.54 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BM014884.D

Acq: 01 May 2018 01:33

Instrument :

BNA_M

ClientSampleId :

F1B67


Tot Ion:163 Resp: 187077

Ion Ratio Lower Upper

163 100

194 3.6 3.5 5.3

164 10.3 8.2 12.4

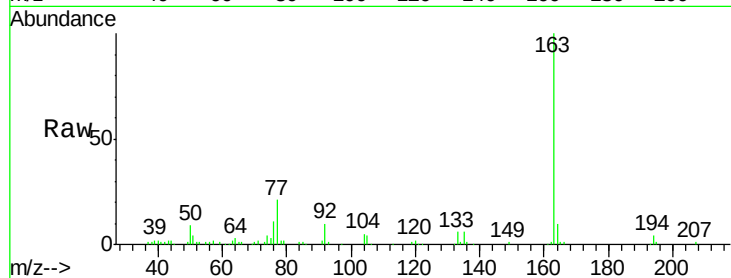

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

