

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
 Data File : BM014885.D
 Acq On : 01 May 2018 02:09
 Operator : SJ/JU
 Sample : J2603-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F1B68

Quant Time: May 01 03:44:58 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 01 03:41:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	397698	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1605661	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	773952	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1537849	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1483491	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1558256	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.64	96	54107	5.94	ng/uL	0.00
5) Phenol-d5	7.62	99	942389	30.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	641401	32.53	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	786030	30.56	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	699843	28.54	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	345751	29.78	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	349212	30.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	639831	27.24	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	889511	38.37	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	1777206	29.42	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2137551	28.65	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	263338	23.49	ng/ul	0.00
57) Fluorene-d10	16.08	176	1502374	28.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	190640	22.91	ng/ul	0.00
70) Anthracene-d10	17.91	188	2159634	30.13	ng/ul	0.00
76) Pyrene-d10	20.15	212	2254334	32.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.23	264	2516559	32.87	ng/ul	0.00
Target Compounds						
6) Phenol	7.65	94	98082	3.242	ng/ul#	86
44) Dimethylphthalate	14.54	163	428192	7.332	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM043018\
Data File : BM014885.D
Acq On : 01 May 2018 02:09
Operator : SJ/JU
Sample : J2603-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F1B68

Quant Time: May 01 03:44:58 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 01 03:41:22 2018
Response via : Initial Calibration

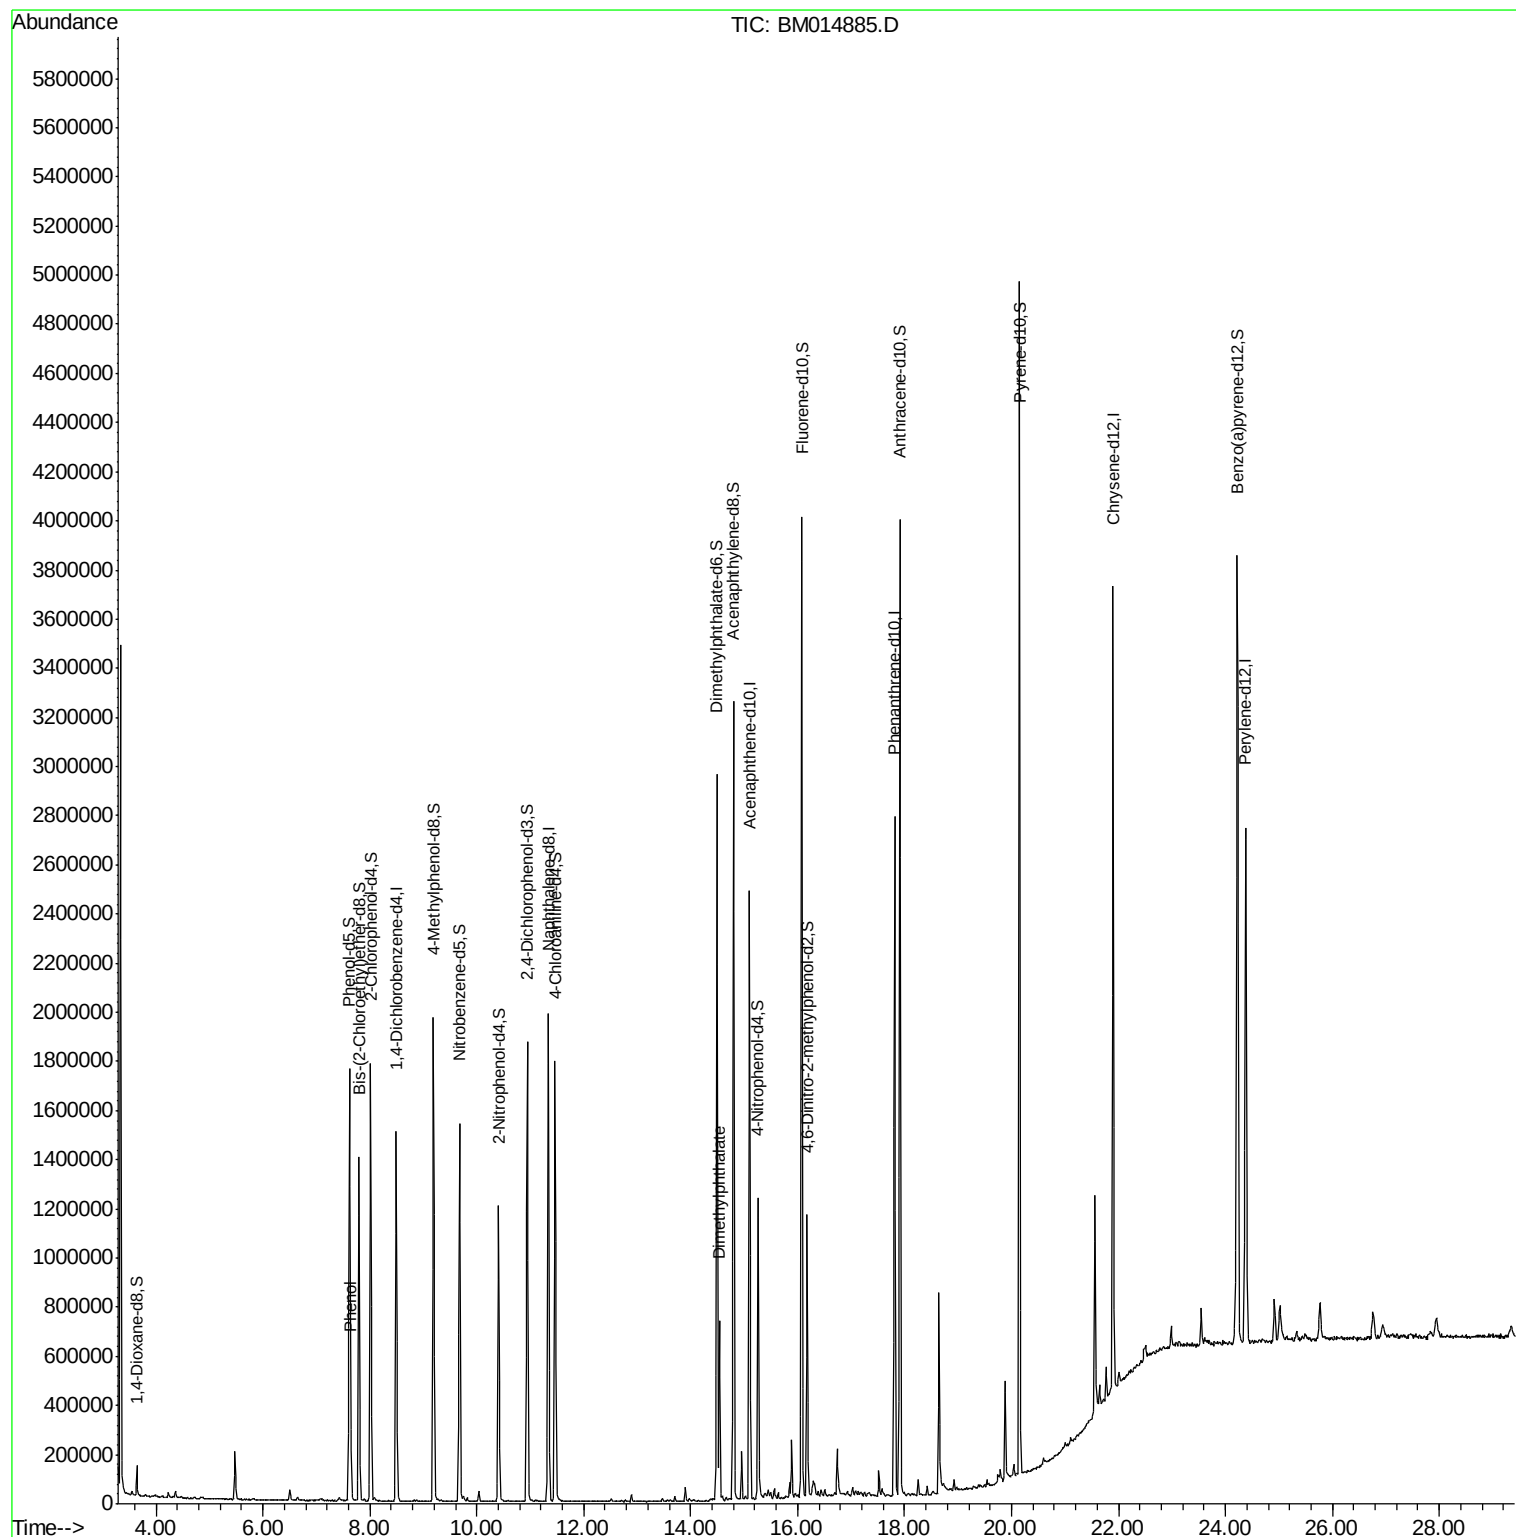

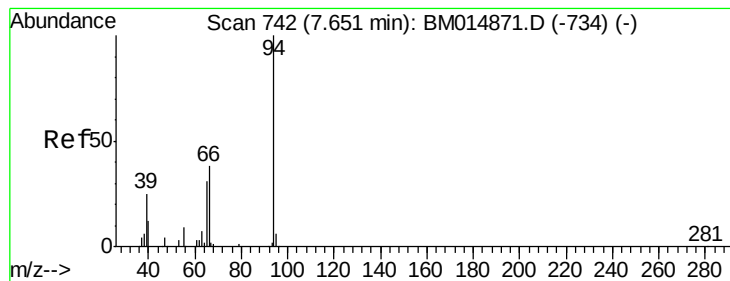

#6

Phenol

Concen: 3.242 ng/ul

RT: 7.65 min Scan# 741

Delta R.T. -0.01 min

Lab File: BM014885.D

Acq: 01 May 2018 02:09

Instrument :

BNA_M

ClientSampleId :

F1B68





Tot Ion: 94 Resp: 98082

Ion Ratio Lower Upper

94 100

65 33.3 28.2 42.4

66 43.5 47.2 70.8#

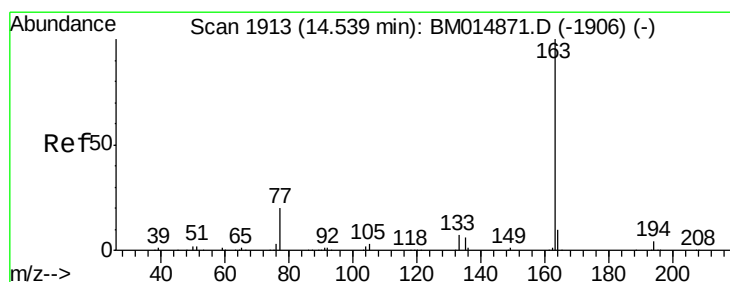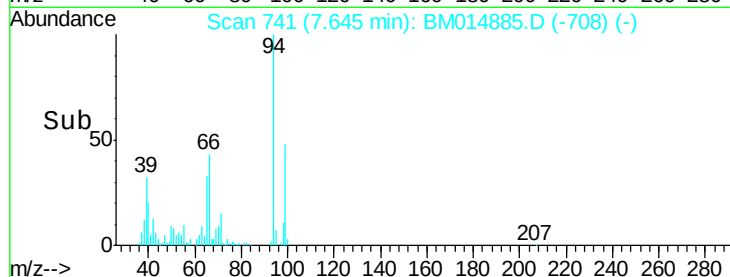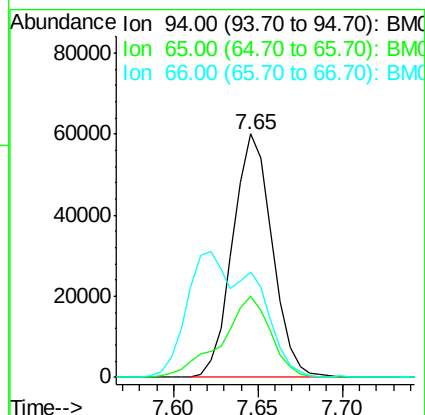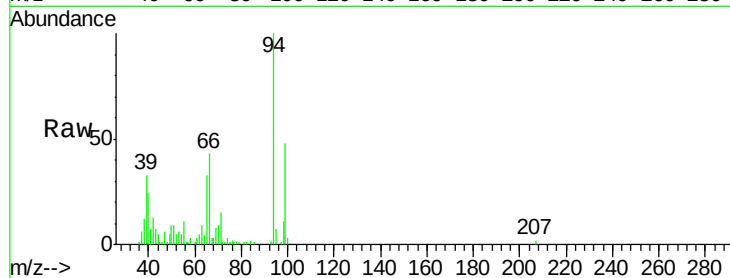

#44

Dimethylphthalate

Concen: 7.332 ng/ul

RT: 14.54 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BM014885.D

Acq: 01 May 2018 02:09

Tgt Ion:163 Resp: 428192

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.8 8.2 12.4

