


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM043019\
 Data File : BM020076.D
 Acq On : 30 Apr 2019 15:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

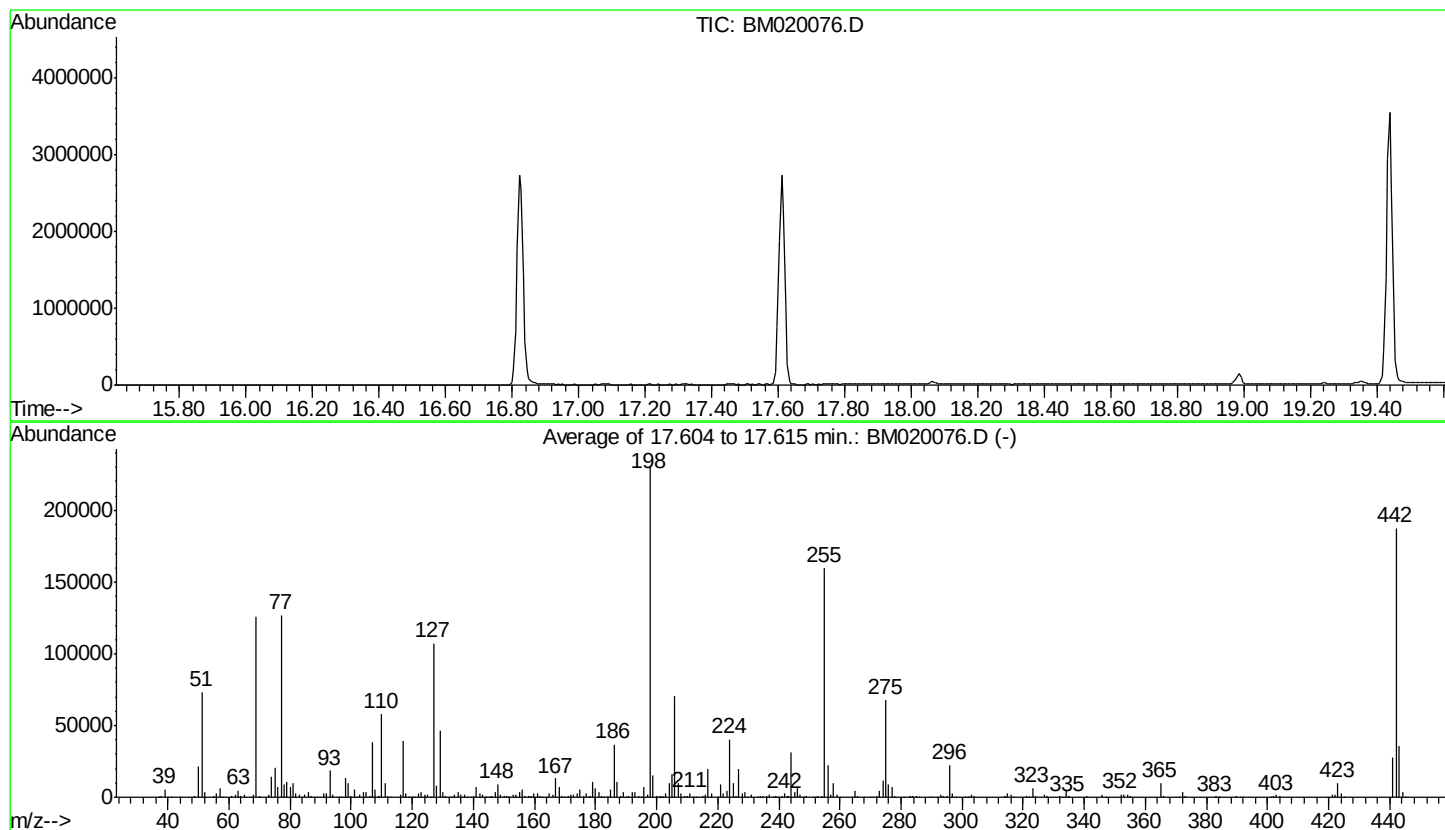

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	73525	PASS
68	69	0.00	2	1.7	2139	PASS
69	198	0.00	100	54.3	125554	PASS
70	69	0.00	2	0.5	619	PASS
127	198	10	80	46.5	107466	PASS
197	198	0.00	2	0.7	1733	PASS
198	198	100	100	100.0	231146	PASS
199	198	5	9	6.7	15529	PASS
275	198	10	60	29.4	67957	PASS
365	198	1	100	4.3	10006	PASS
441	198	0.01	100	12.0	27818	PASS
442	198	50	100	81.2	187765	PASS
443	442	15	24	18.8	35330	PASS