
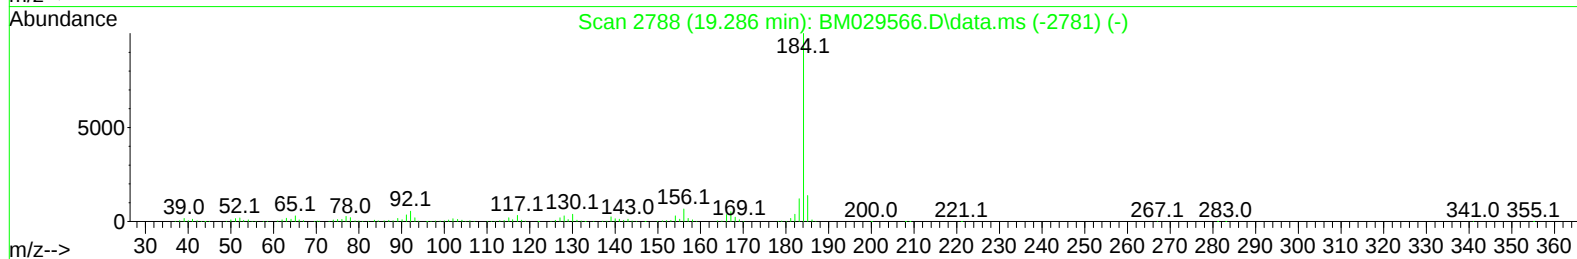
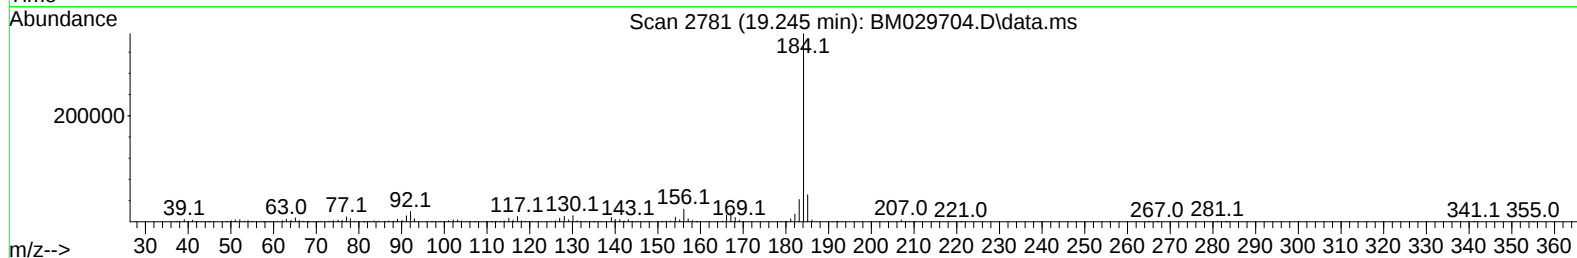


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
 Data File : BM029704.D
 Acq On : 29 Apr 2021 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 11:54:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 28 17:58:02 2021
 Response via : Initial Calibration

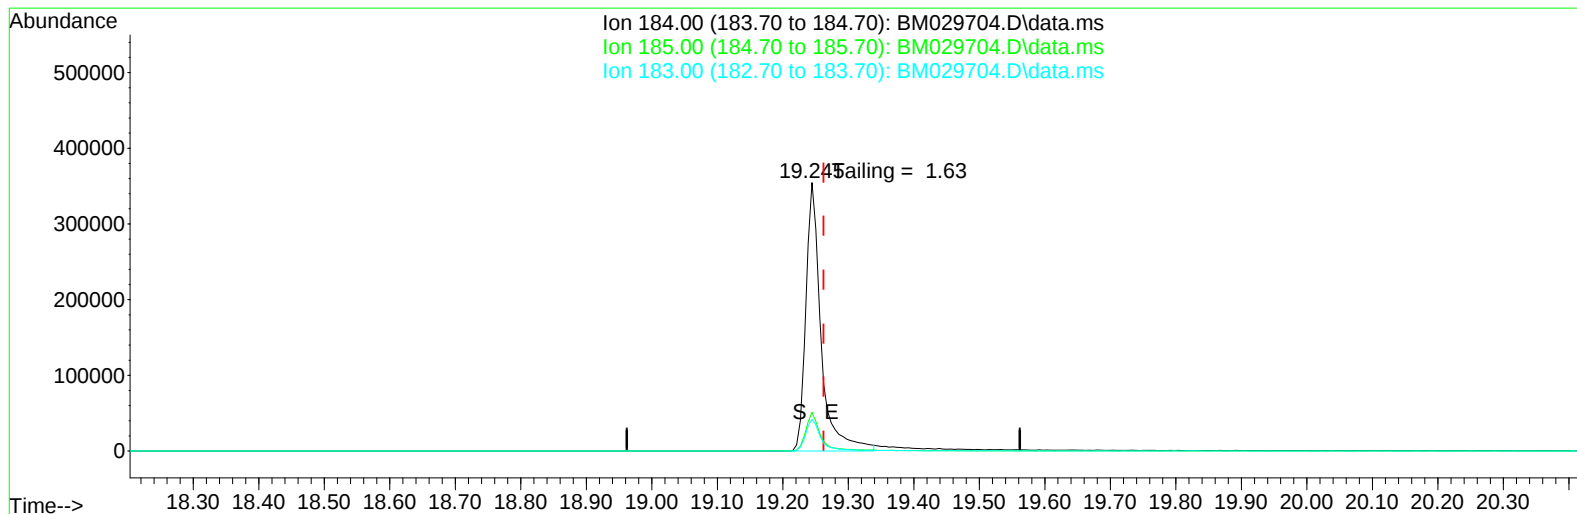

TIC: BM029704.D\data.ms

(77) Benzidine




19.245min (-0.018) 0.00 ng

response 593886

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.45
183.00	12.30	11.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
 Data File : BM029704.D
 Acq On : 29 Apr 2021 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 11:54:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 28 17:58:02 2021
 Response via : Initial Calibration

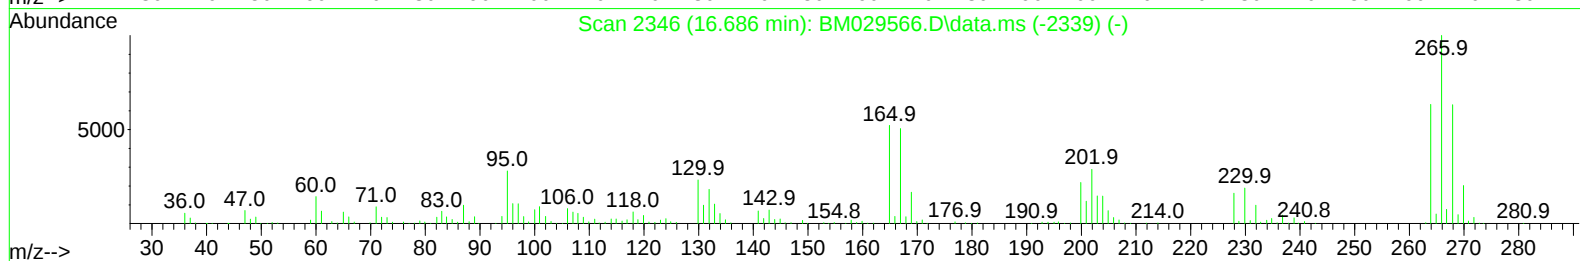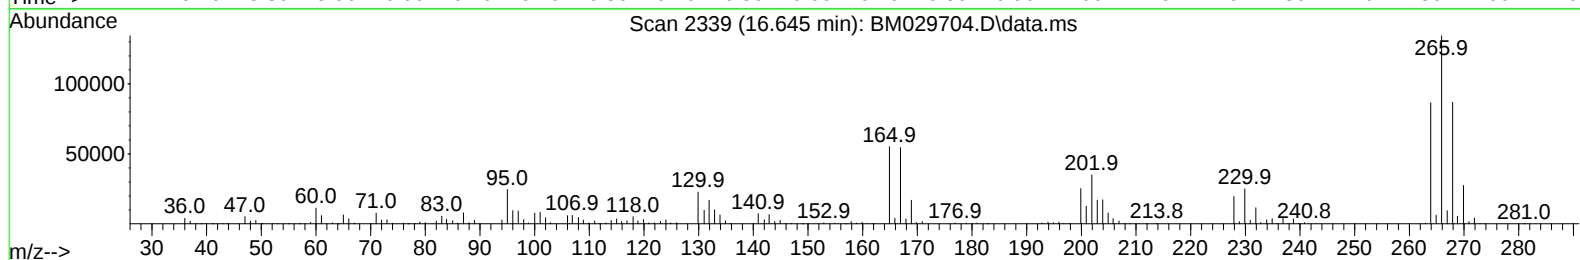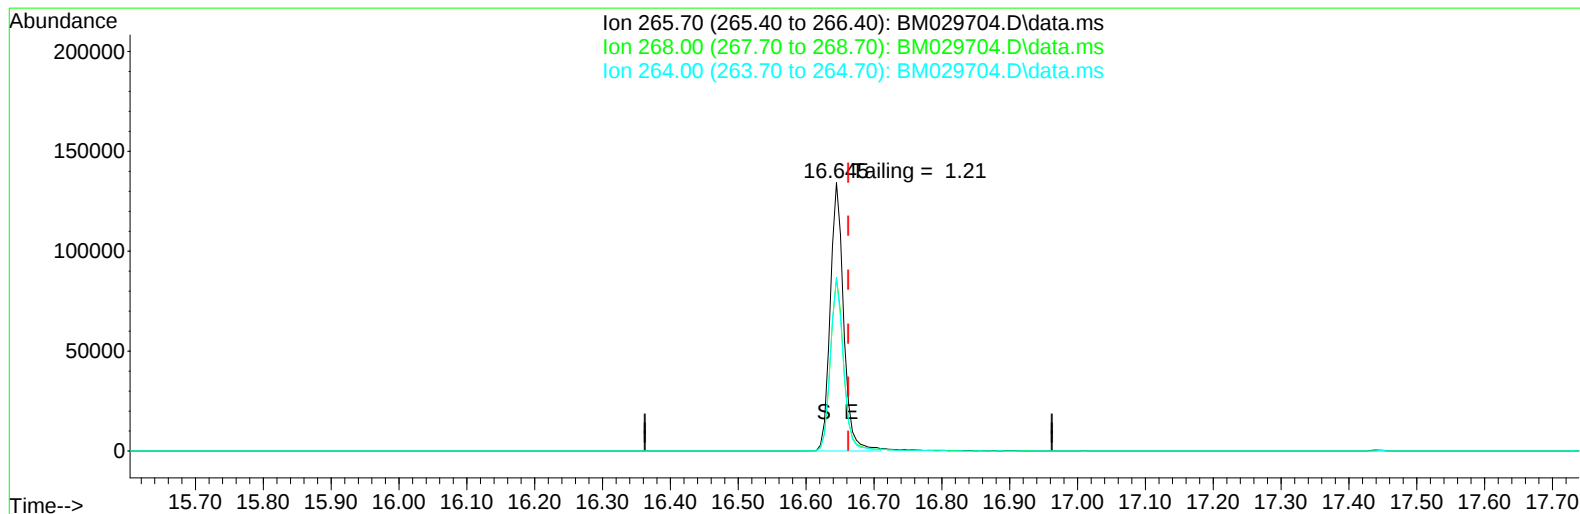

TIC: BM029704.D\data.ms

(70) Pentachlorophenol (C)

16.645min (-0.018) 0.00 ng

response 185543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.66
264.00	64.90	64.42
0.00	0.00	0.00