
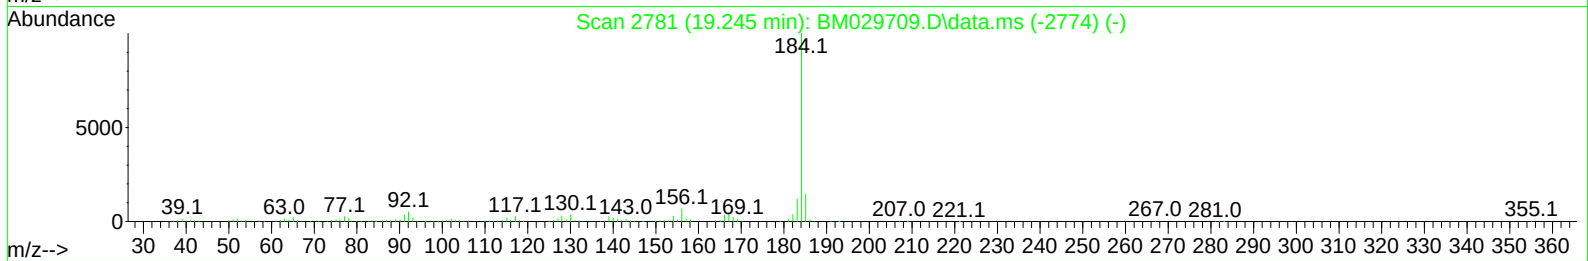
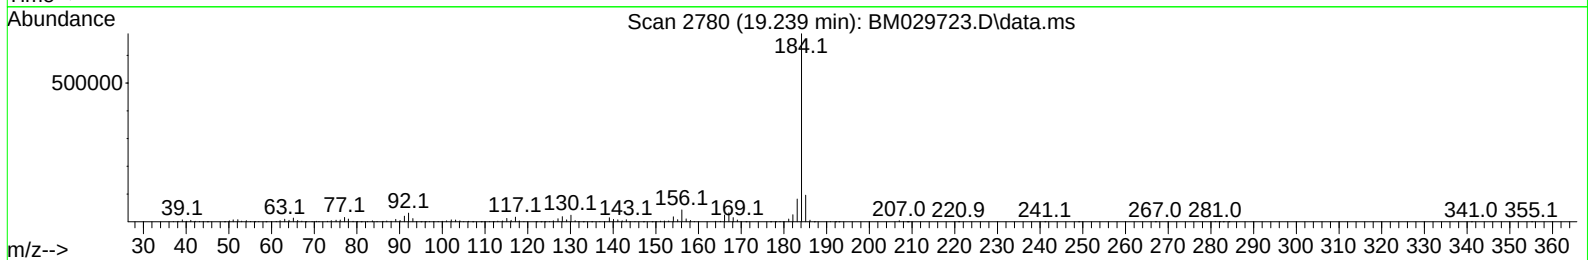


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
 Data File : BM029723.D
 Acq On : 30 Apr 2021 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 12:41:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 17:34:54 2021
 Response via : Initial Calibration

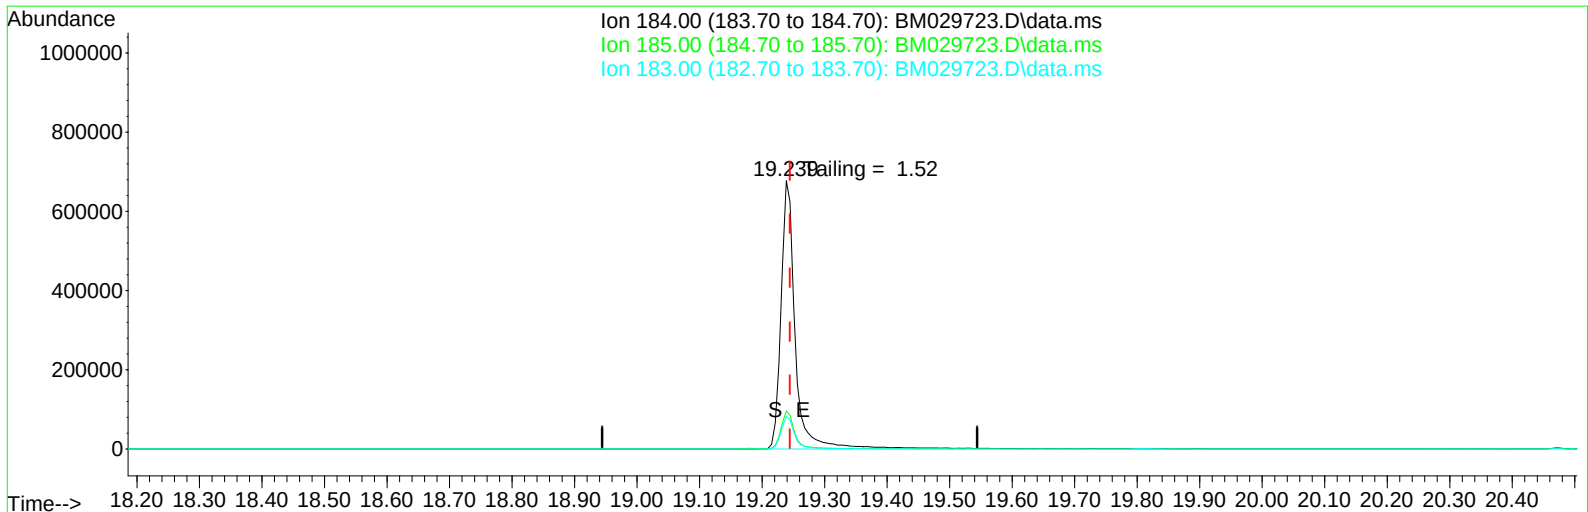

TIC: BM029723.D\data.ms

(77) Benzidine




19.239min (-0.006) 951361.01 ng

response 1073428

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.18
183.00	12.30	12.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
 Data File : BM029723.D
 Acq On : 30 Apr 2021 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 12:41:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 29 17:34:54 2021
 Response via : Initial Calibration

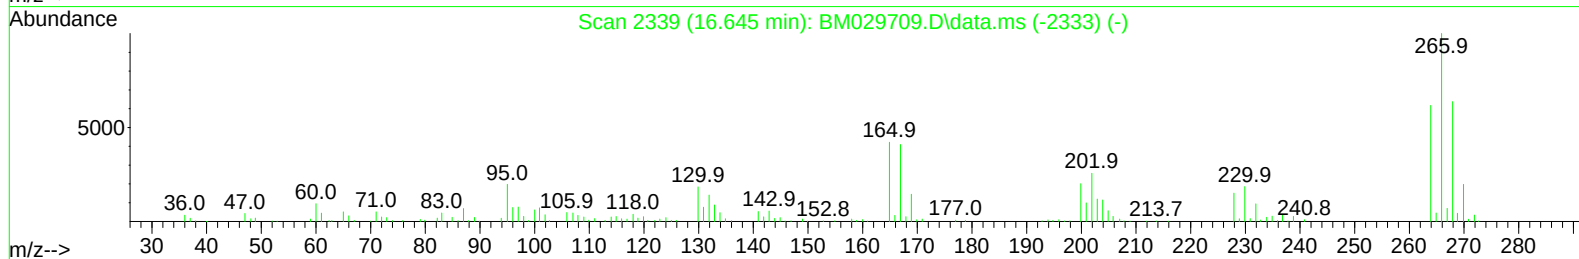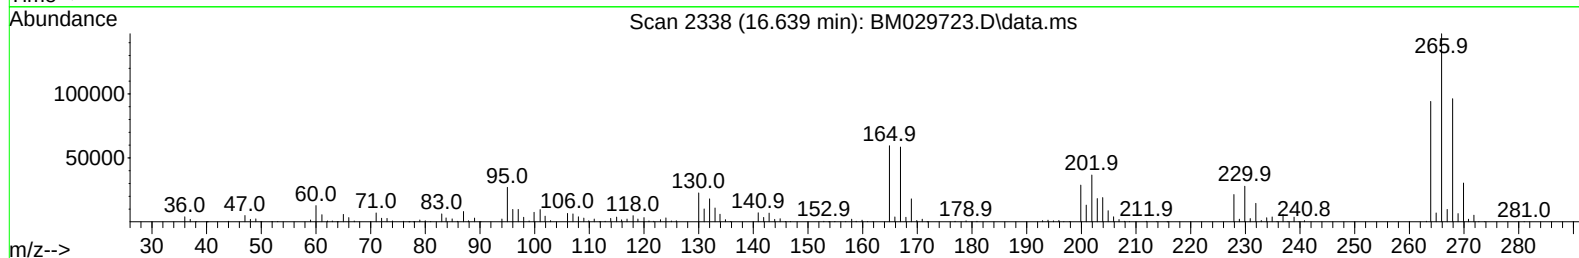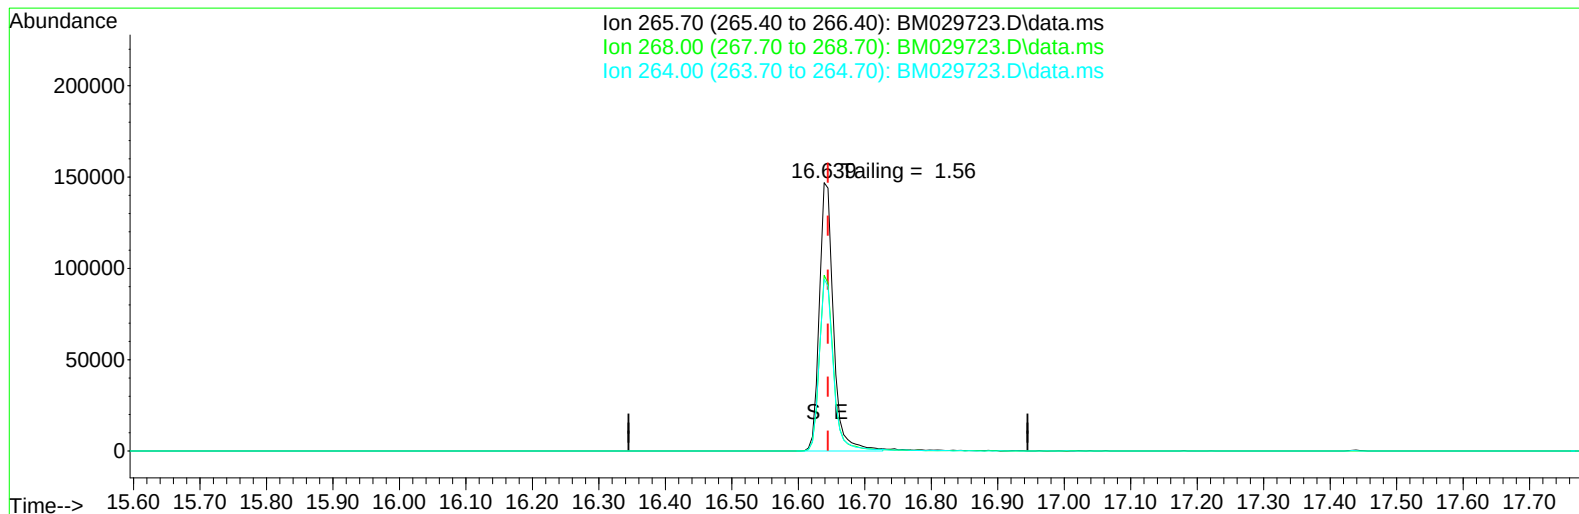

TIC: BM029723.D\data.ms

(70) Pentachlorophenol (C)

16.639min (-0.006) 0.00 ng

response 219351

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	65.49
264.00	64.90	64.03
0.00	0.00	0.00