

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
 Data File : BM029727.D
 Acq On : 30 Apr 2021 13:37
 Operator : CG/JU
 Sample : PB136086BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB136086BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	385	392	410	rBV	1304793	1875796	30.29%	7.857%
2	6.781	654	662	688	rBV	1185835	1923380	31.05%	8.057%
3	7.592	793	800	813	rBV	270014	432433	6.98%	1.811%
4	8.745	988	996	1015	rBV	739710	1297496	20.95%	5.435%
5	10.369	1265	1272	1287	rBV	329707	574255	9.27%	2.405%
6	12.857	1688	1695	1715	rBV	2764591	4054401	65.46%	16.983%
7	14.239	1923	1930	1943	rBV	632319	951250	15.36%	3.985%
8	15.733	2178	2184	2207	rBV	2414761	3347156	54.04%	14.021%
9	16.986	2390	2397	2411	rBV	735361	1110962	17.94%	4.654%
10	19.621	2839	2845	2861	rBV	5249038	6193787	100.00%	25.945%
11	21.168	3103	3108	3120	rBV	826182	1088610	17.58%	4.560%
12	23.344	3471	3478	3486	rBV2	518673	1023348	16.52%	4.287%




Sum of corrected areas: 23872874

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
Data File : BM029727.D
Acq On : 30 Apr 2021 13:37
Operator : CG/JU
Sample : PB136086BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

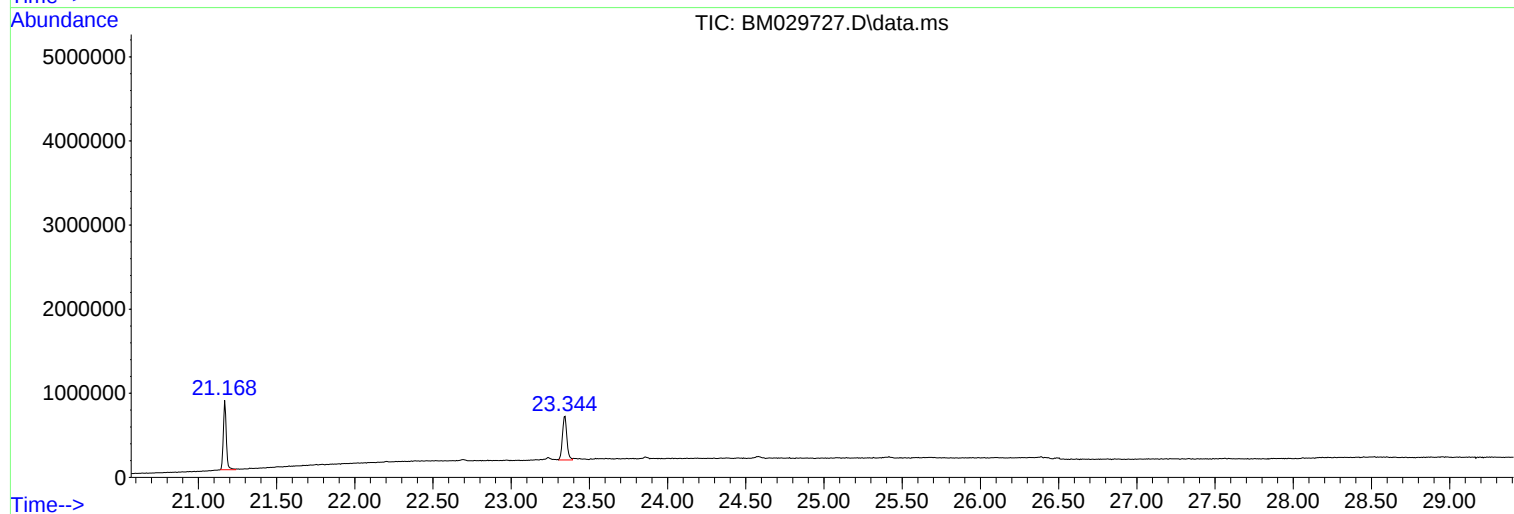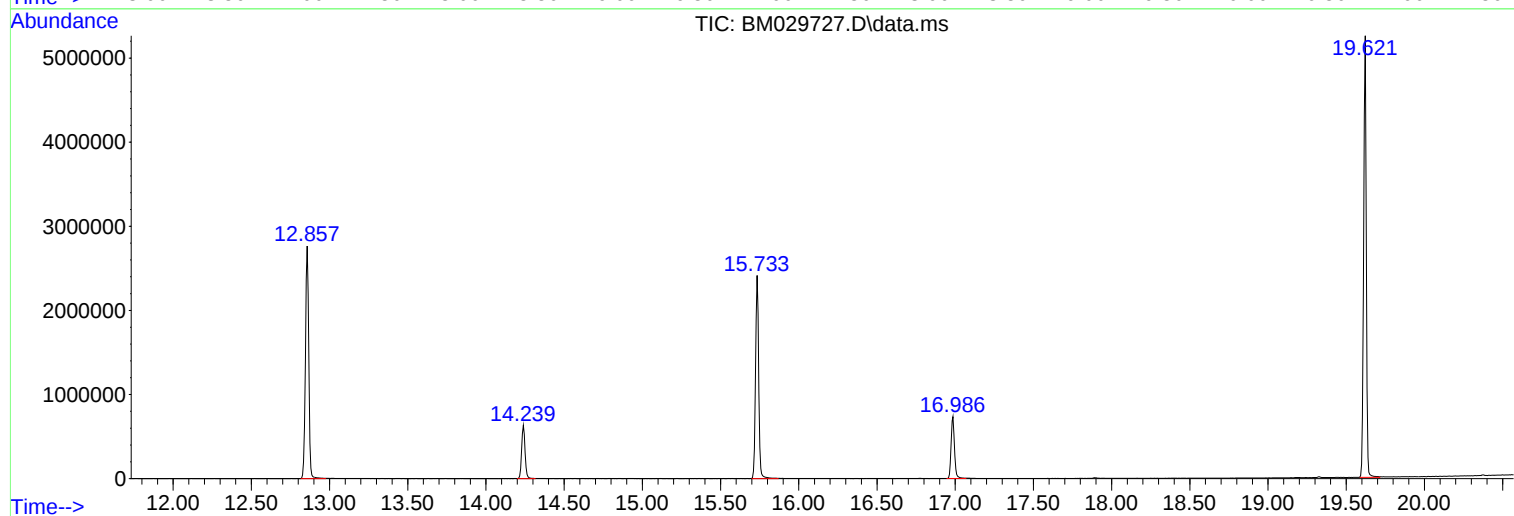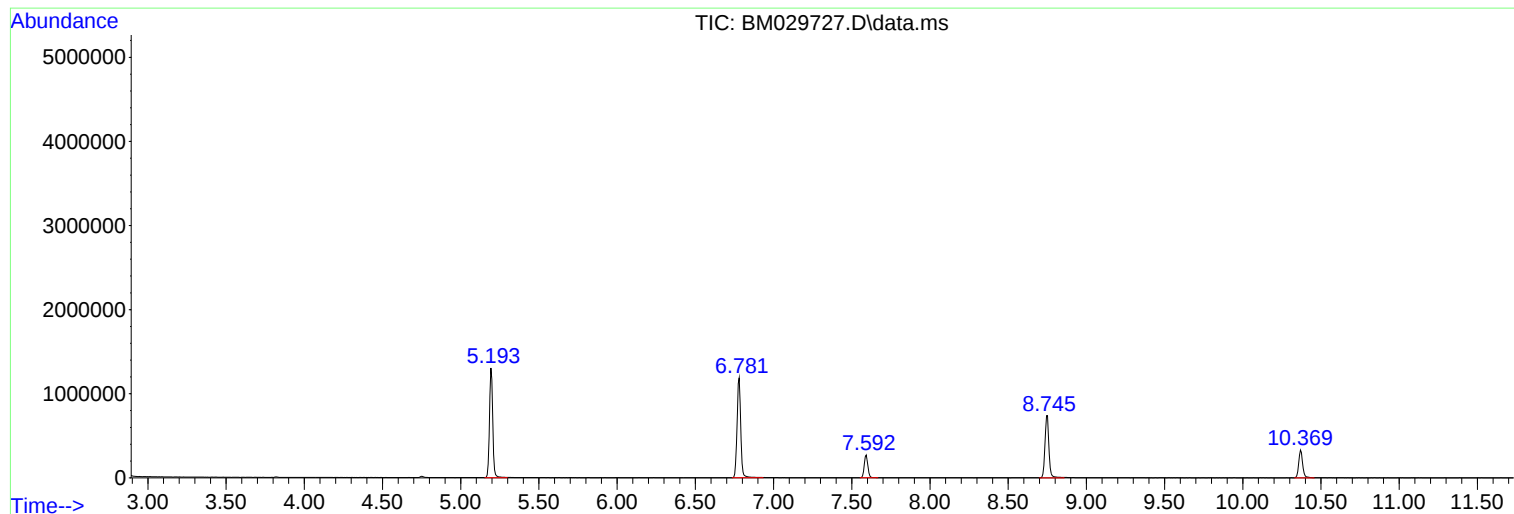

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
Data File : BM029727.D
Acq On : 30 Apr 2021 13:37
Operator : CG/JU
Sample : PB136086BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
Data File : BM029727.D
Acq On : 30 Apr 2021 13:37
Operator : CG/JU
Sample : PB136086BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------