


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
 Data File : BM029704.D
 Acq On : 29 Apr 2021 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 29 17:34:54 2021

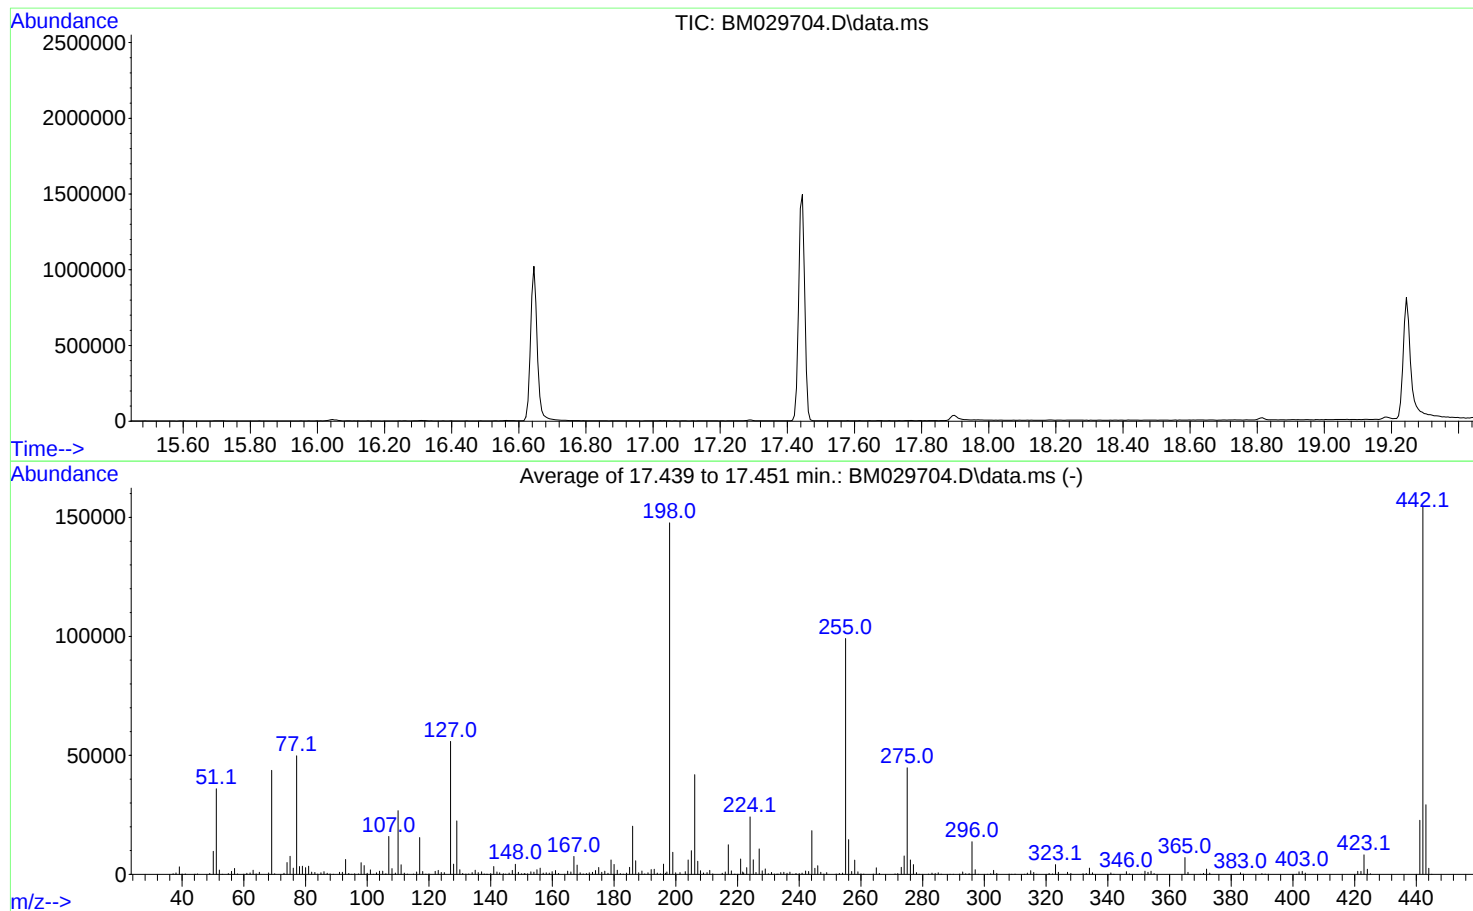




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	35997	PASS
68	69	0.00	2	1.3	581	PASS
69	198	0.00	100	29.6	43693	PASS
70	69	0.00	2	0.7	310	PASS
127	198	10	80	37.8	55856	PASS
197	198	0.00	2	0.7	1035	PASS
198	198	100	100	100.0	147688	PASS
199	198	5	9	6.3	9283	PASS
275	198	10	60	30.3	44795	PASS
365	198	1	100	4.8	7039	PASS
441	198	0.01	100	15.4	22757	PASS
442	442	50	100	100.0	154560	PASS
443	442	15	24	18.9	29227	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
Data File : BM029704.D
Acq On : 29 Apr 2021 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 29 11:54:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 28 17:58:02 2021
Response via : Initial Calibration

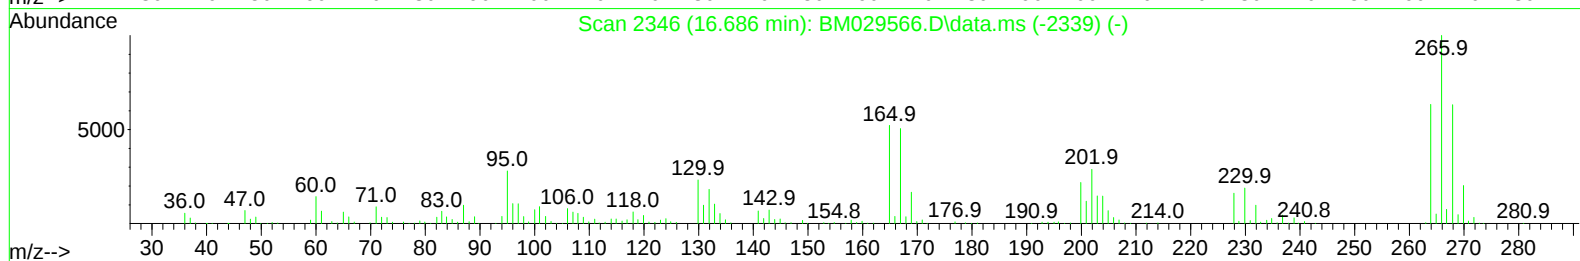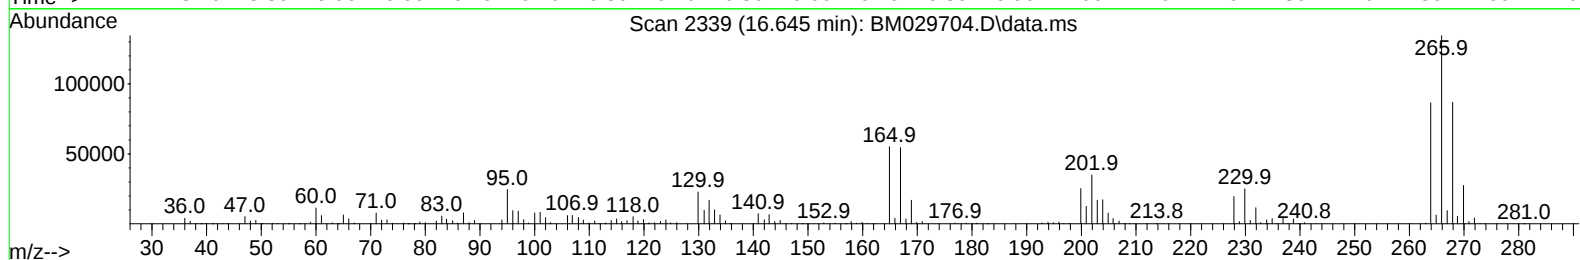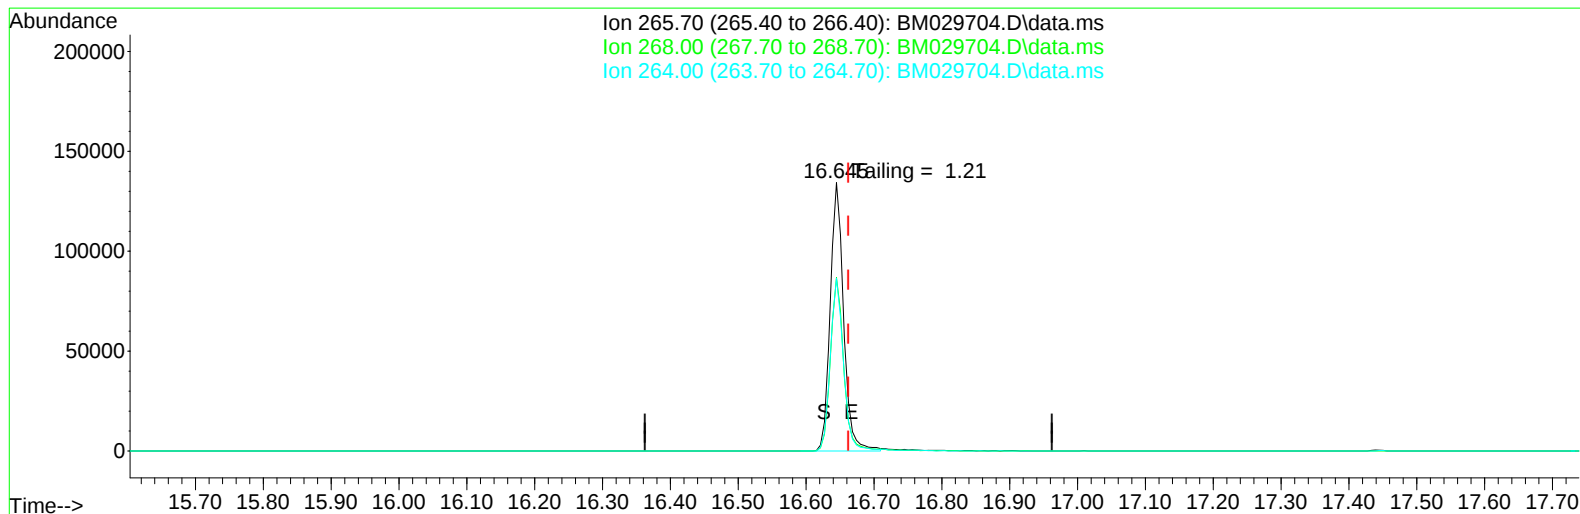

TIC: BM029704.D\data.ms

(70) Pentachlorophenol (C)

16.645min (-0.018) 0.00 ng

response 185543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.66
264.00	64.90	64.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/30/2021	BNA_M	<u>BM029704.D</u>
Compound Name	Response	Retention Time
DDT	613237	20.48
DDD	1895	20.03
DDE	875	19.52
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2770	616007	0.45

Instrument :
BNA_M
ClientSampleId :
DFTPP