


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
 Data File : BM029723.D
 Acq On : 30 Apr 2021 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 29 17:34:54 2021

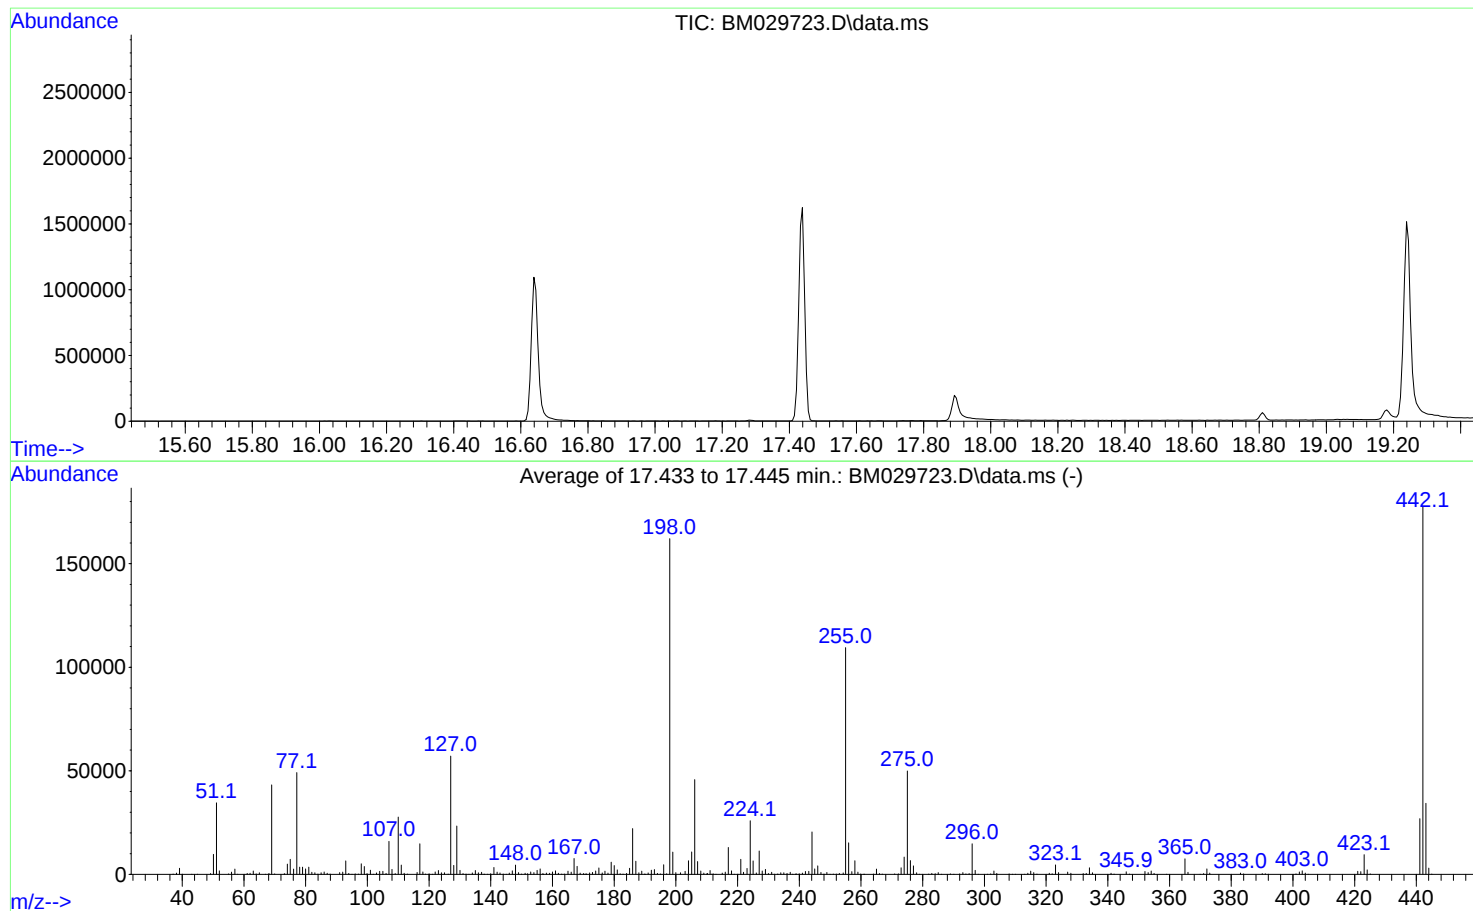




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.3	34525	PASS
68	69	0.00	2	1.1	456	PASS
69	198	0.00	100	26.6	43171	PASS
70	69	0.00	2	0.5	205	PASS
127	198	10	80	35.2	57093	PASS
197	198	0.00	2	0.2	291	PASS
198	198	100	100	100.0	162123	PASS
199	198	5	9	6.6	10774	PASS
275	198	10	60	30.8	49872	PASS
365	198	1	100	4.6	7519	PASS
441	198	0.01	100	16.6	26867	PASS
442	442	50	100	100.0	177621	PASS
443	442	15	24	19.3	34323	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\
Data File : BM029723.D
Acq On : 30 Apr 2021 10:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 30 12:41:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 29 17:34:54 2021
Response via : Initial Calibration

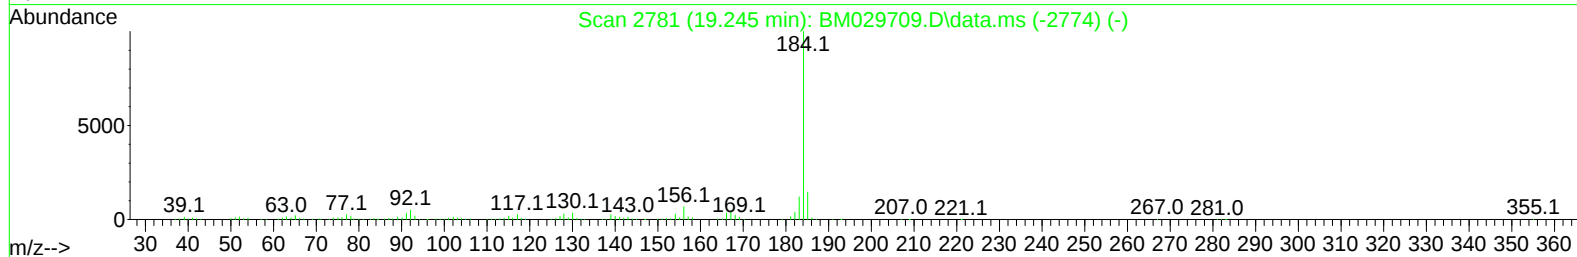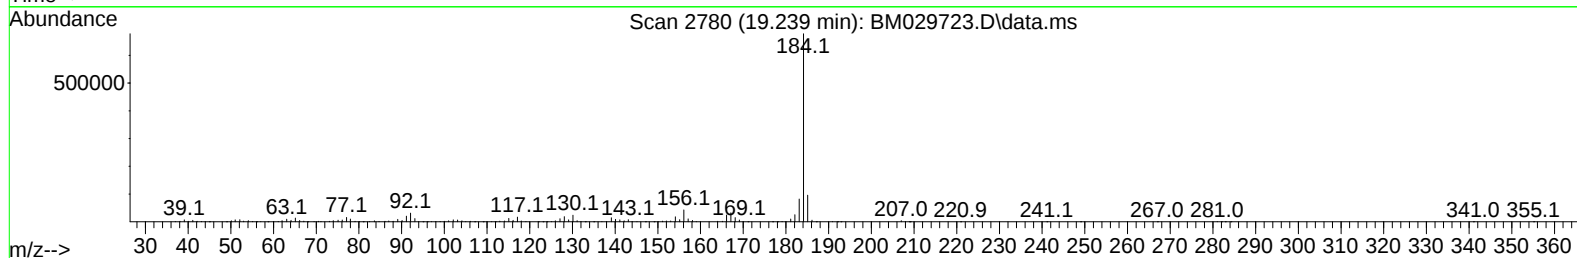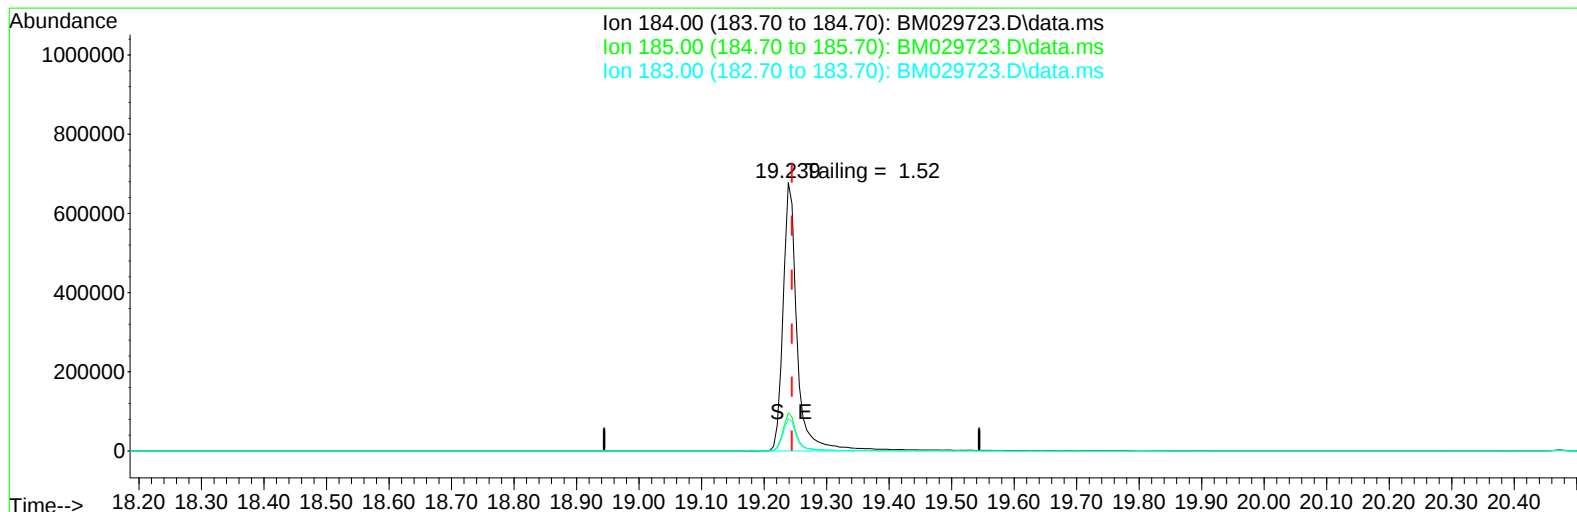

TIC: BM029723.D\data.ms

(77) Benzidine

19.239min (-0.006) 951361.01 ng




response 1073428

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.18
183.00	12.30	12.14
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043021\  
Data File : BM029723.D  
Acq On    : 30 Apr 2021  10:35  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 30 12:41:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 29 17:34:54 2021
Response via : Initial Calibration

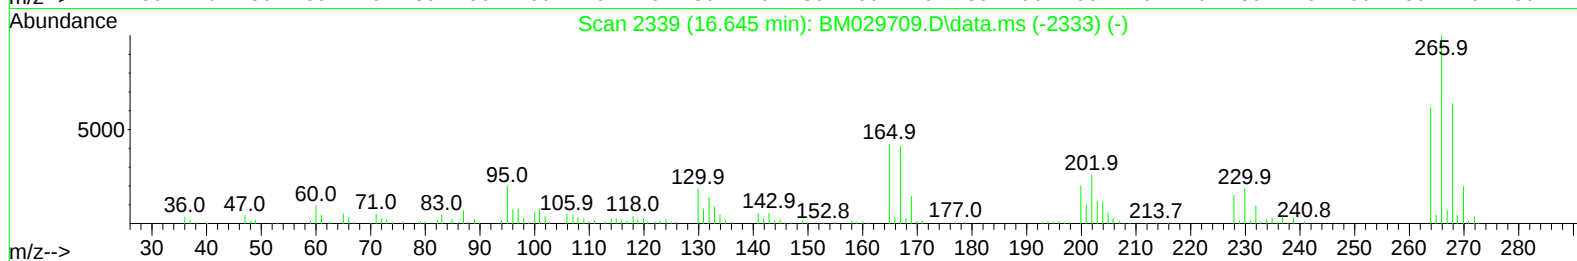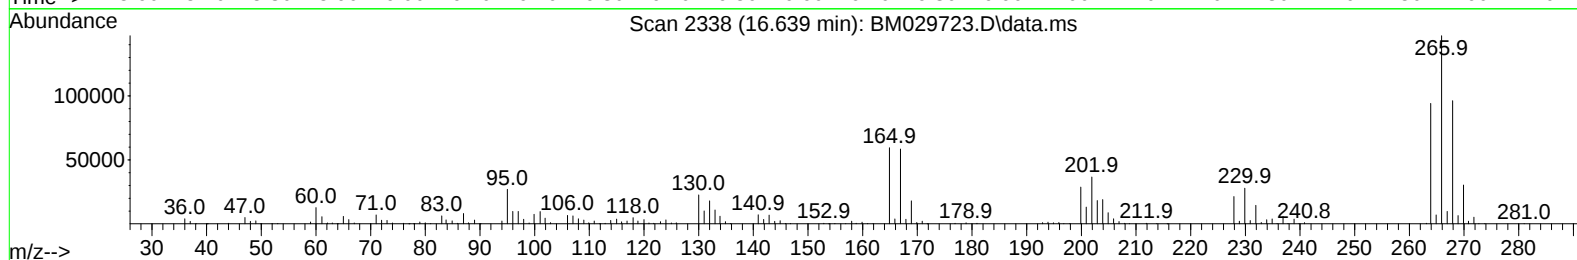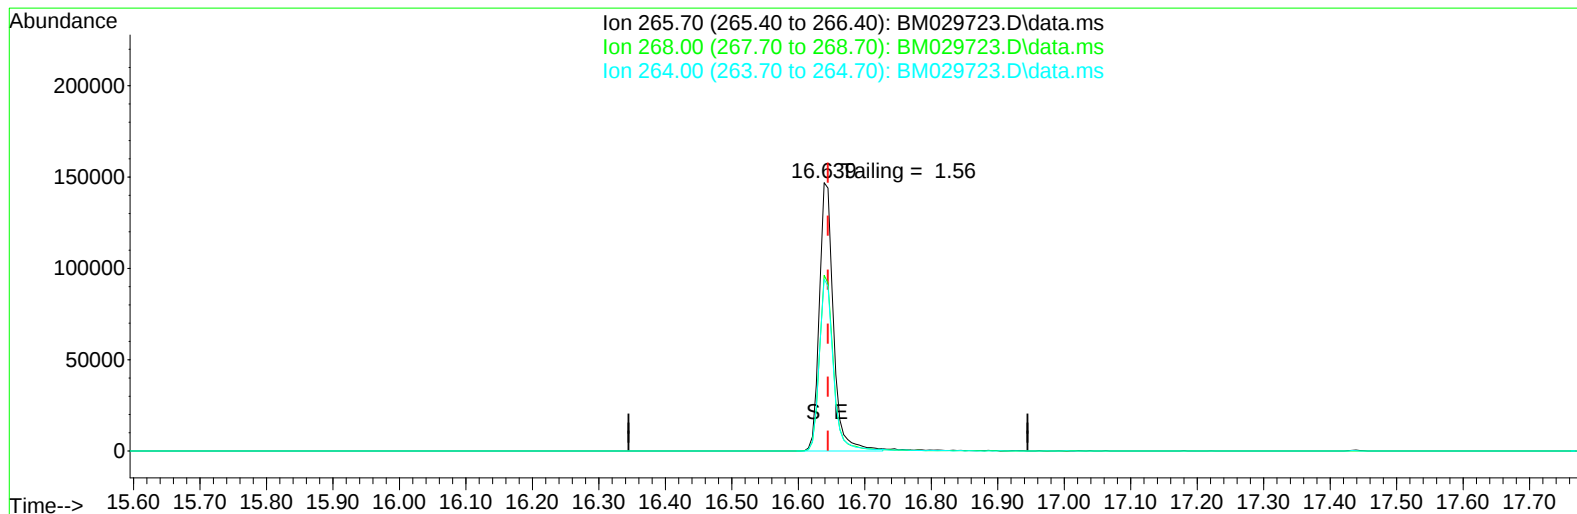

TIC: BM029723.D\data.ms

(70) **Pentachlorophenol (C)**

16.639min (-0.006) 0.00 ng

response **219351**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	65.49
264.00	64.90	64.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/30/2021	BNA_M	<u>BM029723.D</u>
Compound Name	Response	Retention Time
DDT	718507	20.47
DDD	3797	20.03
DDE	907	19.53
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4704	723211	0.65

Instrument :
BNA_M
ClientSampleId :
DFTPP