
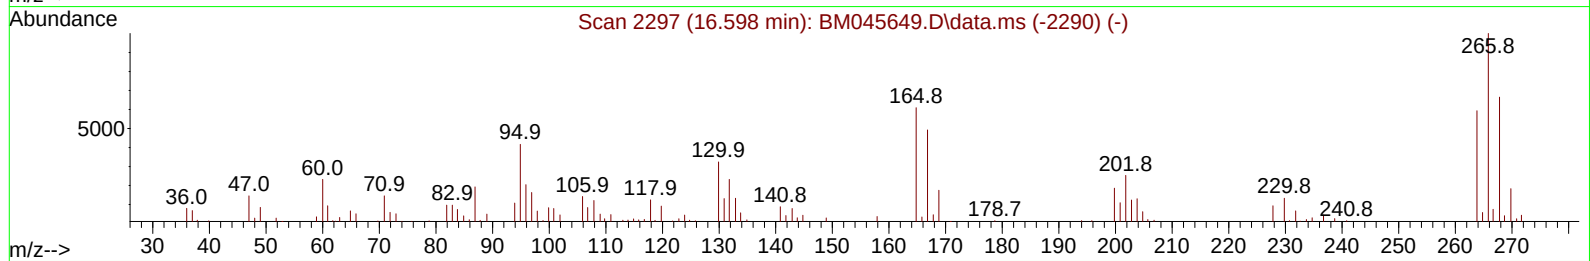
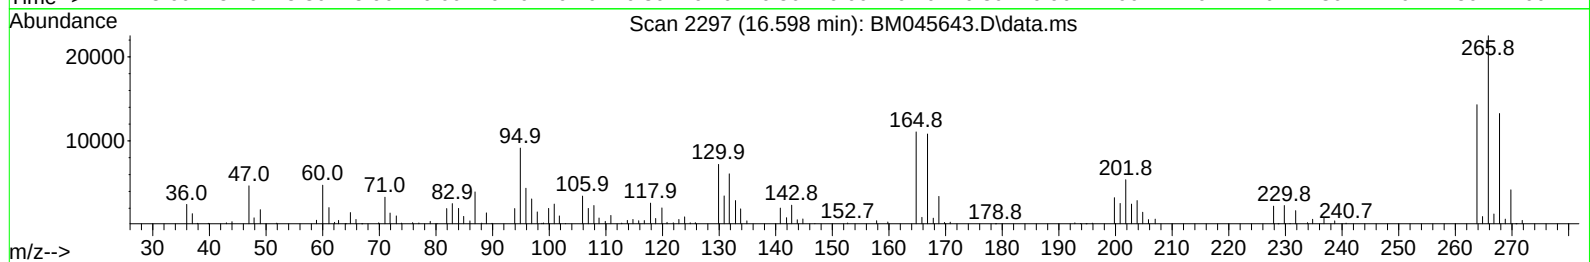


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
Data File : BM045643.D
Acq On : 30 Apr 2024 13:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 14:36:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 06:17:41 2024
Response via : Initial Calibration

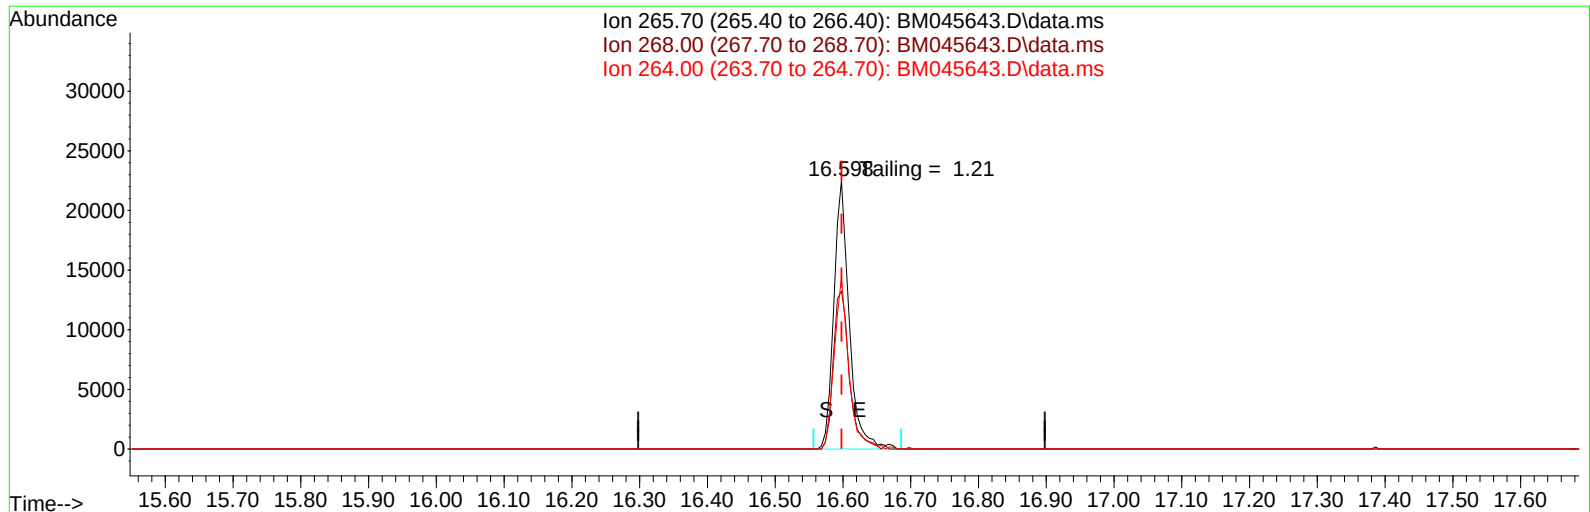

TIC: BM045643.D\data.ms

(70) Pentachlorophenol (C)




16.598min (-0.000) 0.00 ng

response 35531

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.70	58.89
264.00	59.40	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
Data File : BM045643.D
Acq On : 30 Apr 2024 13:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 14:36:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 06:17:41 2024
Response via : Initial Calibration

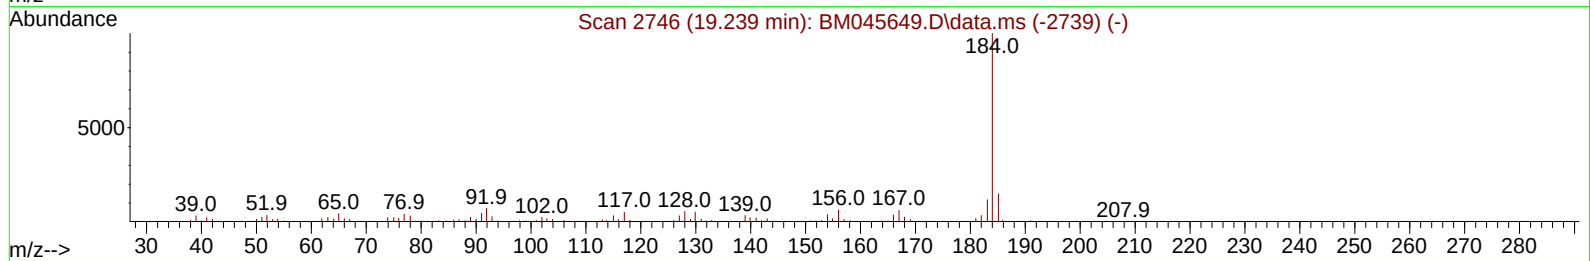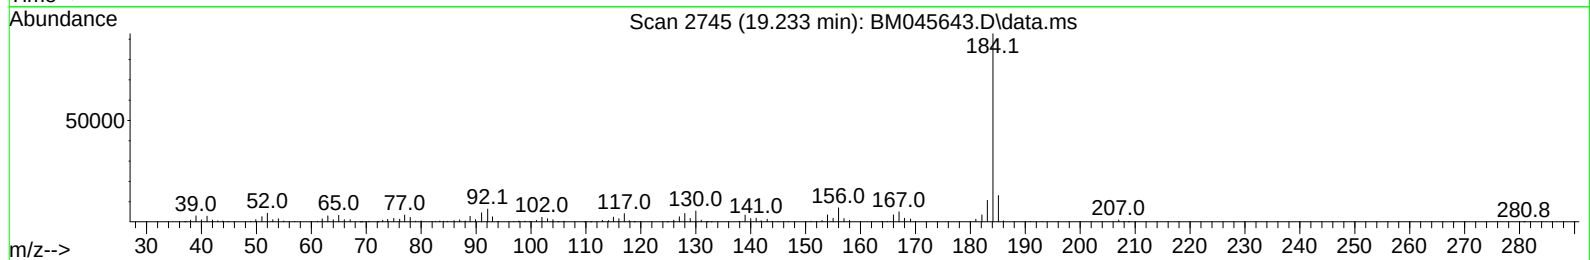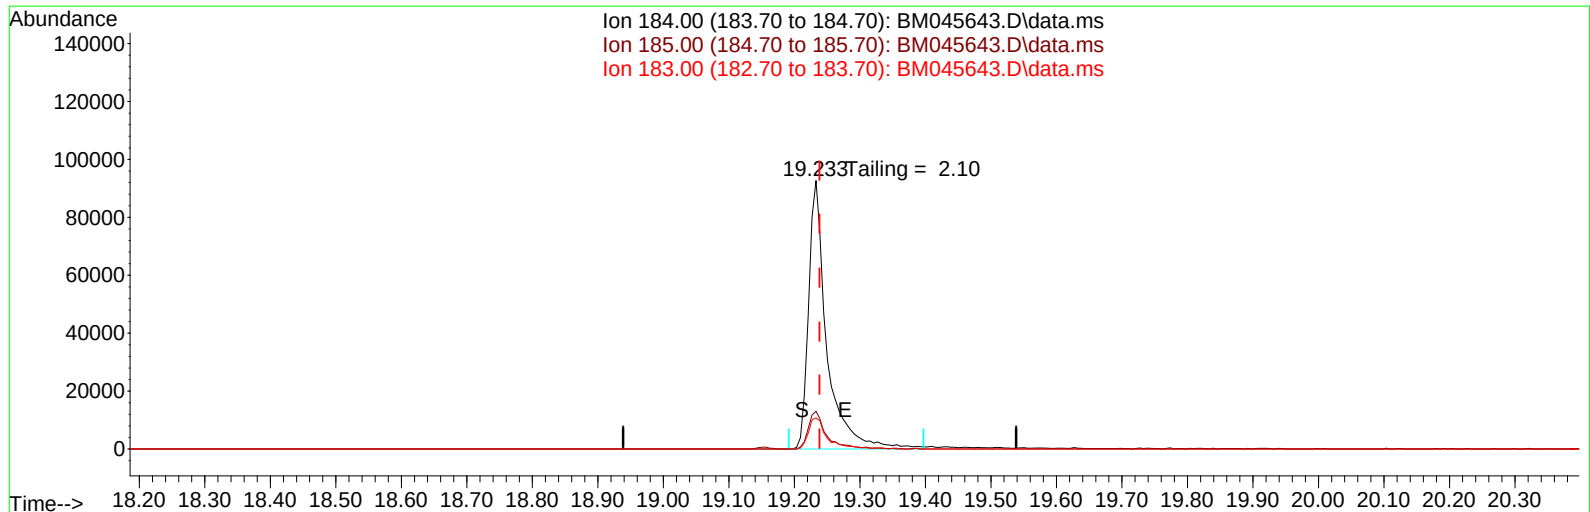

TIC: BM045643.D\data.ms

(77) Benzidine**19.233min (-0.006) 14711.34 ng****response 179365**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.08
183.00	11.70	11.56
0.00	0.00	0.00