

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
 Data File : BM045654.D
 Acq On : 30 Apr 2024 20:46
 Operator : MA/JU
 Sample : PB160479TB
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB160479TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM045654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.151	345	351	364	rBV	545210	757976	80.89%	14.557%
2	6.710	609	616	633	rBV	412321	702374	74.96%	13.489%
3	7.516	747	753	762	rBV	82273	135163	14.42%	2.596%
4	8.687	944	952	965	rBV	210549	395774	42.24%	7.601%
5	10.292	1218	1225	1239	rBV	70772	148826	15.88%	2.858%
6	12.786	1642	1649	1666	rBV	451246	740994	79.08%	14.231%
7	14.180	1877	1886	1897	rBV2	94896	165953	17.71%	3.187%
8	15.686	2136	2142	2159	rBV	331166	526996	56.24%	10.121%
9	16.951	2349	2357	2368	rBV	93806	171592	18.31%	3.295%
10	19.598	2802	2807	2815	rBV	769132	937056	100.00%	17.996%
11	21.168	3069	3074	3082	rBV	137160	215572	23.01%	4.140%
12	23.344	3438	3444	3453	rBV	143822	308754	32.95%	5.930%




Sum of corrected areas: 5207030

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
Data File : BM045654.D
Acq On : 30 Apr 2024 20:46
Operator : MA/JU
Sample : PB160479TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160479TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

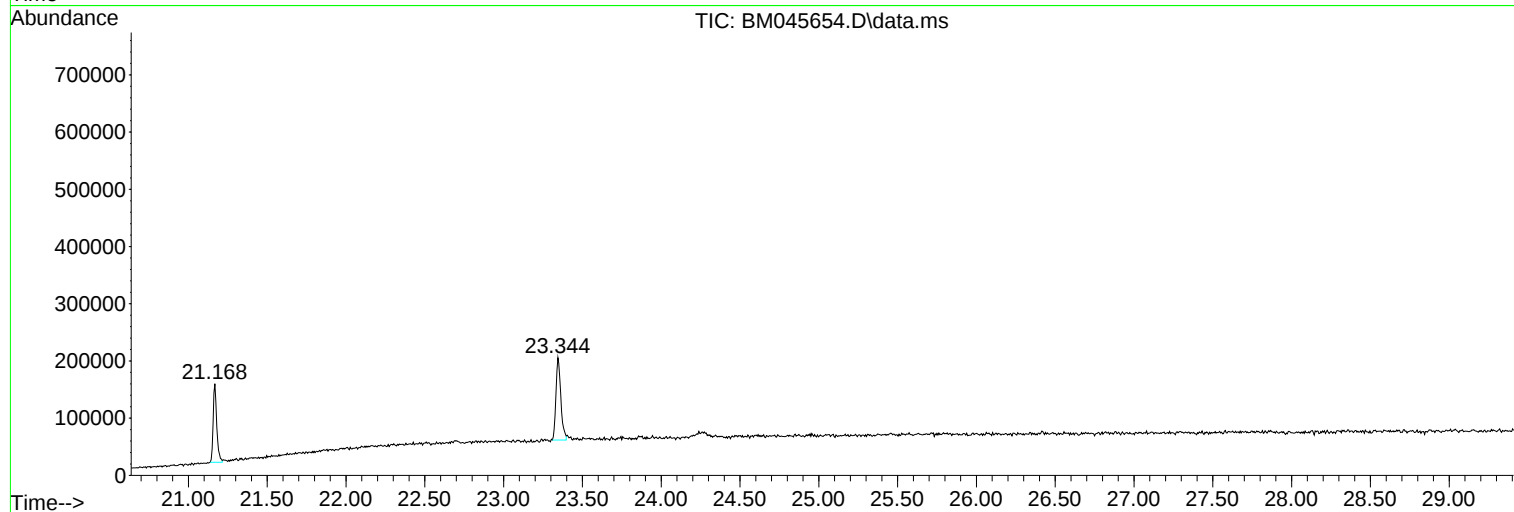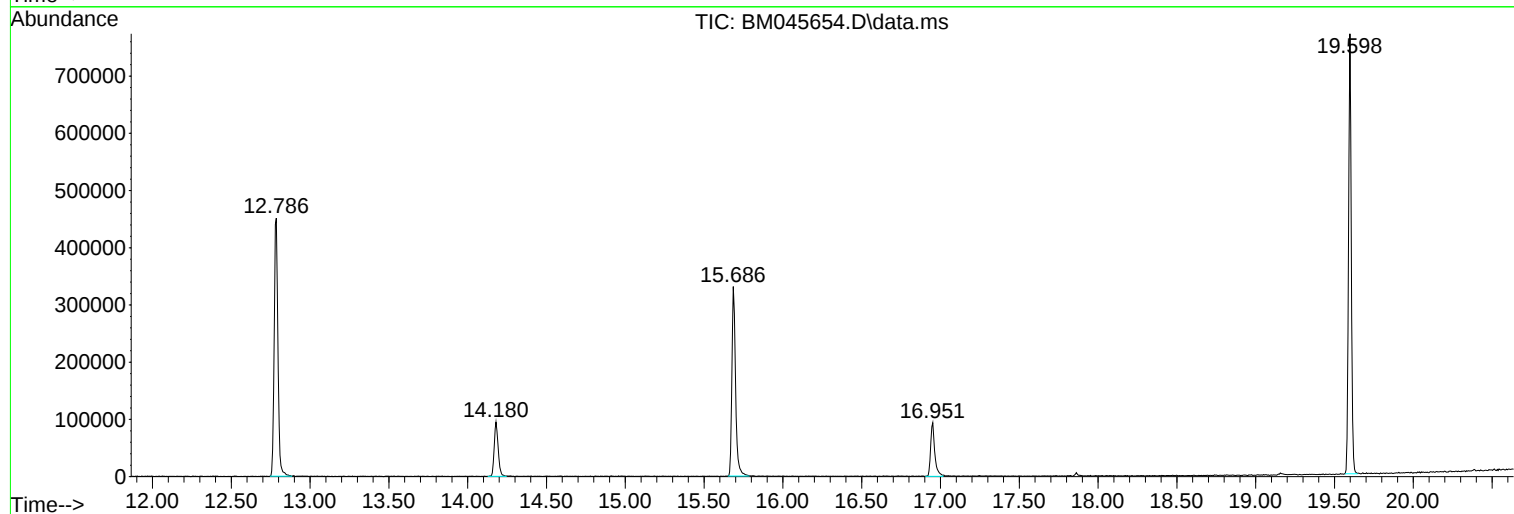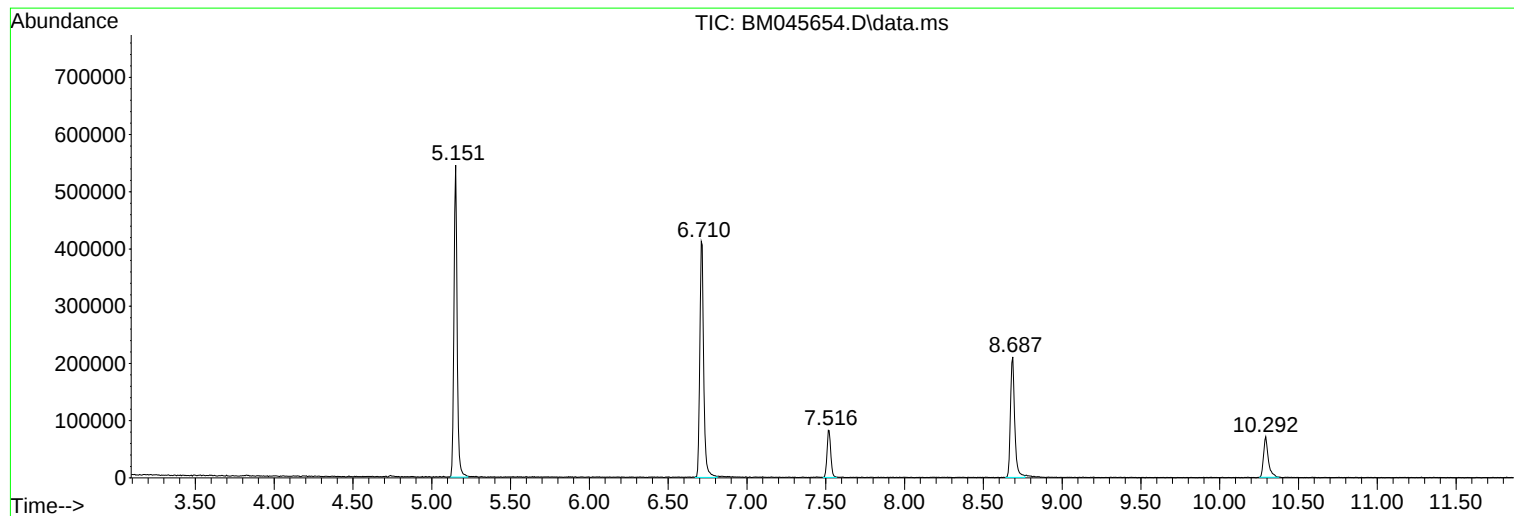

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
Data File : BM045654.D
Acq On : 30 Apr 2024 20:46
Operator : MA/JU
Sample : PB160479TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160479TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
Data File : BM045654.D
Acq On : 30 Apr 2024 20:46
Operator : MA/JU
Sample : PB160479TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160479TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------