
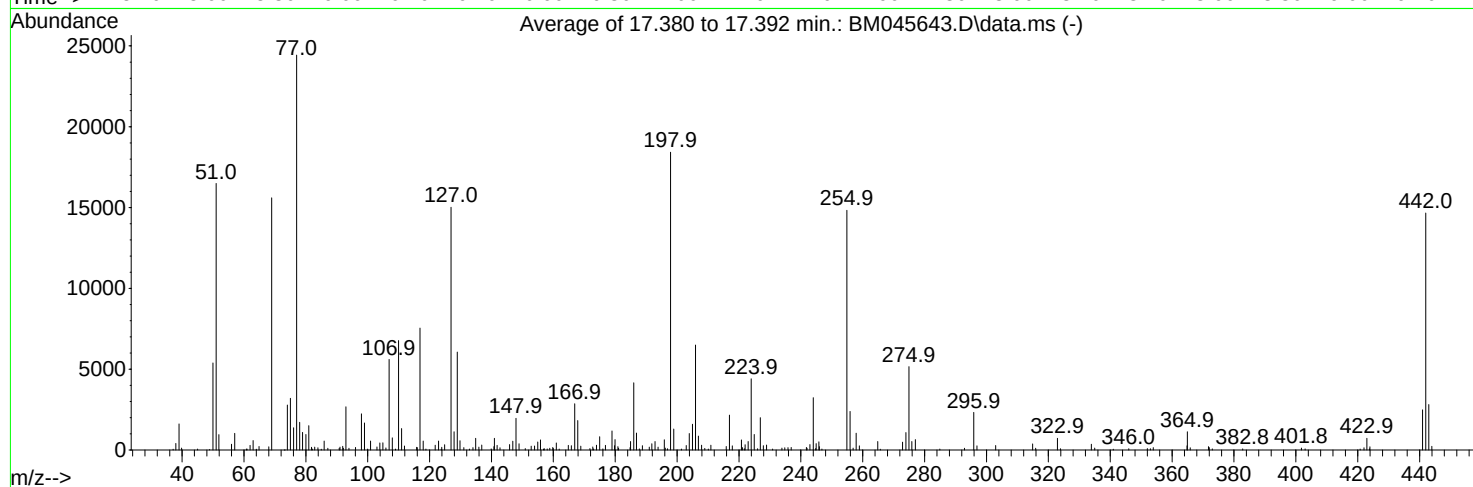


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
Data File : BM045643.D
Acq On : 30 Apr 2024 13:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 11:38:17 2020

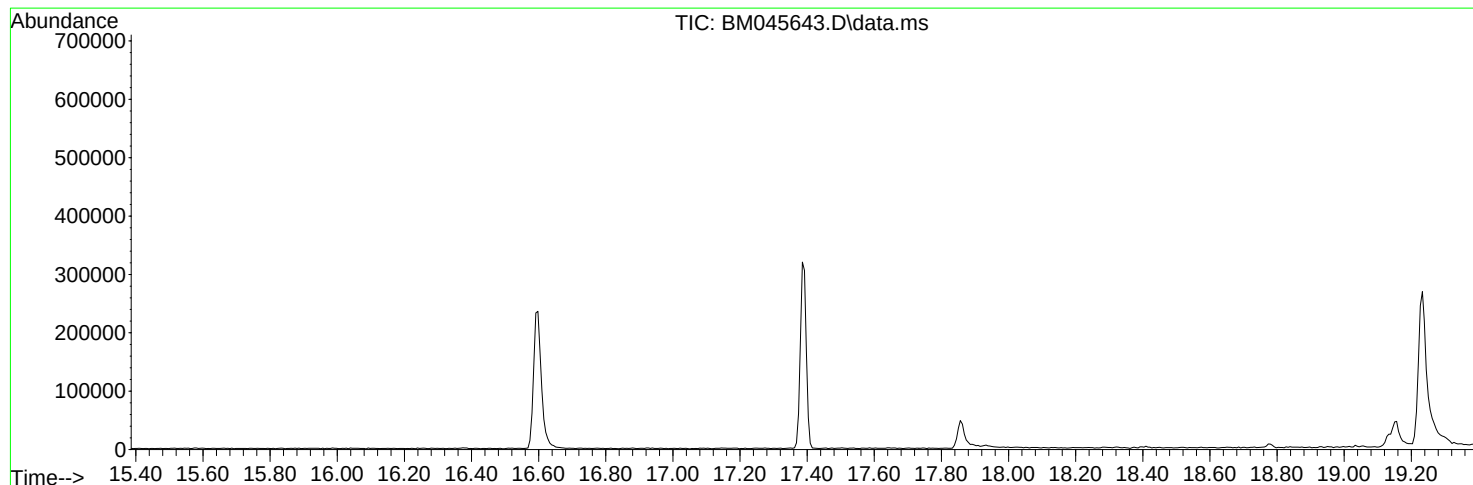




AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2424

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.3	201	PASS
69	69	100	100	100.0	15596	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.4	77	PASS
198	198	100	100	100.0	18420	PASS
199	198	5	9	7.1	1300	PASS
365	198	1	100	6.1	1130	PASS
441	443	0.01	150	88.4	2480	PASS
442	442	100	100	100.0	14663	PASS
443	442	15	24	19.1	2807	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
Data File : BM045643.D
Acq On : 30 Apr 2024 13:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 03 14:36:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 06:17:41 2024
Response via : Initial Calibration

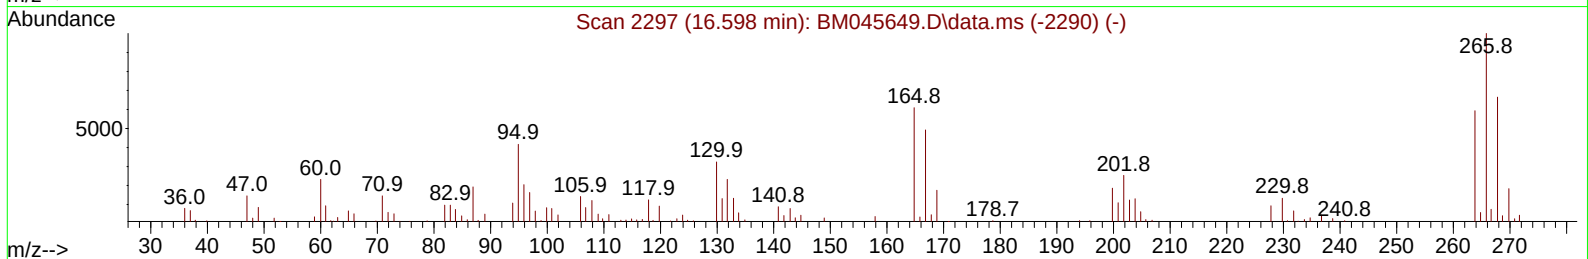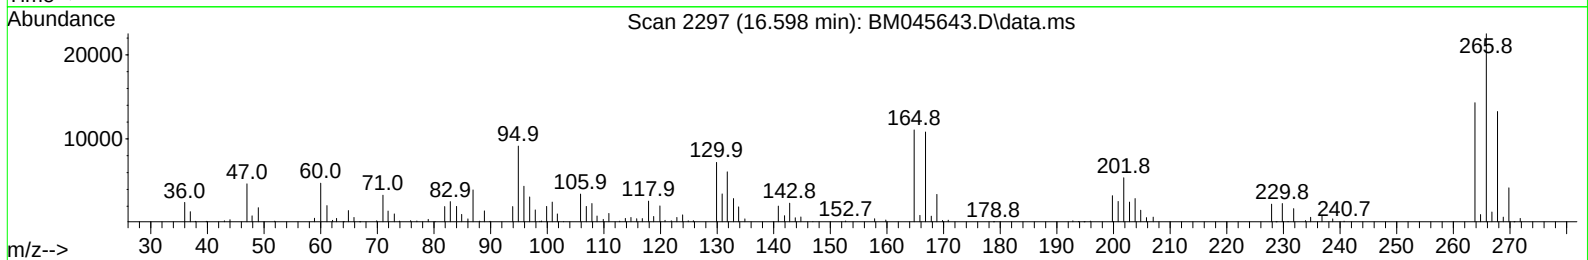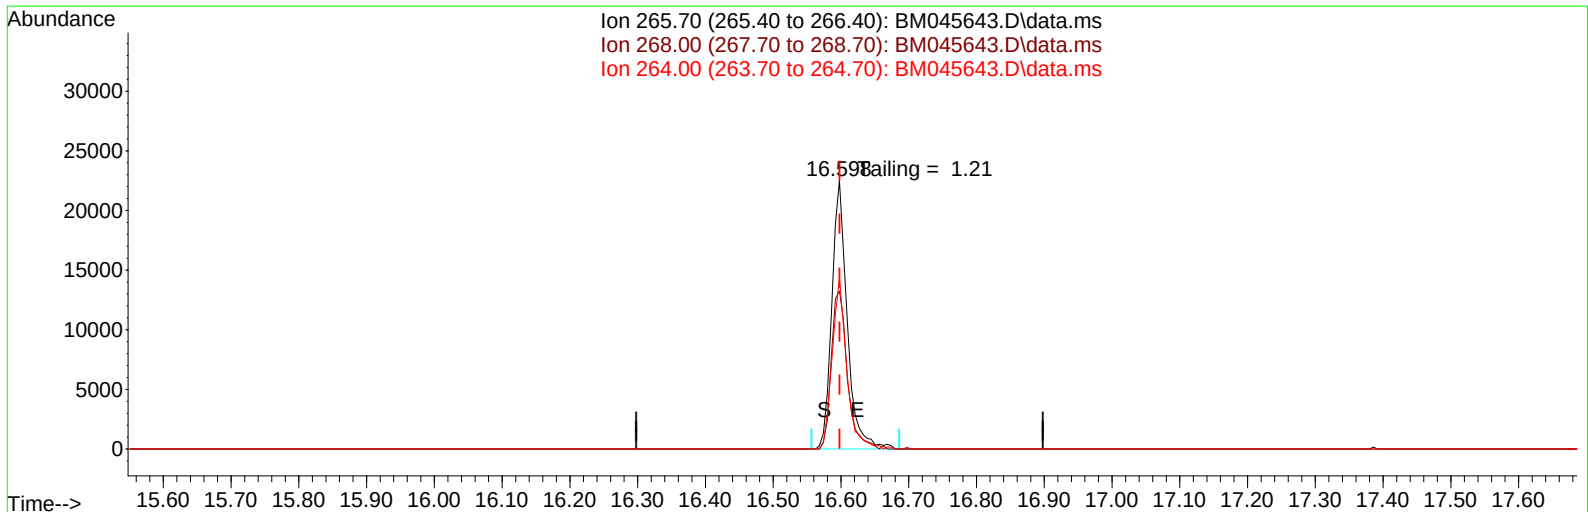

TIC: BM045643.D\data.ms

(70) Pentachlorophenol (C)

16.598min (-0.000) 0.00 ng




response 35531

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.70	58.89
264.00	59.40	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043024\
 Data File : BM045643.D
 Acq On : 30 Apr 2024 13:21
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 03 14:36:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 06:17:41 2024
 Response via : Initial Calibration

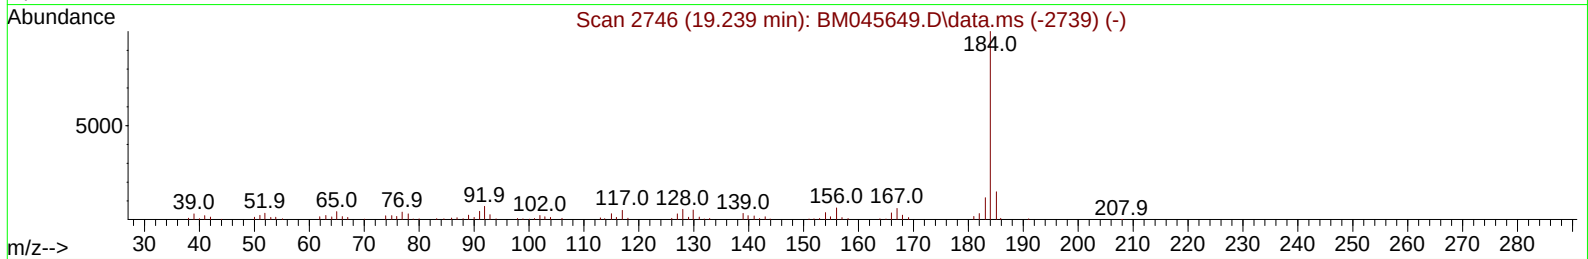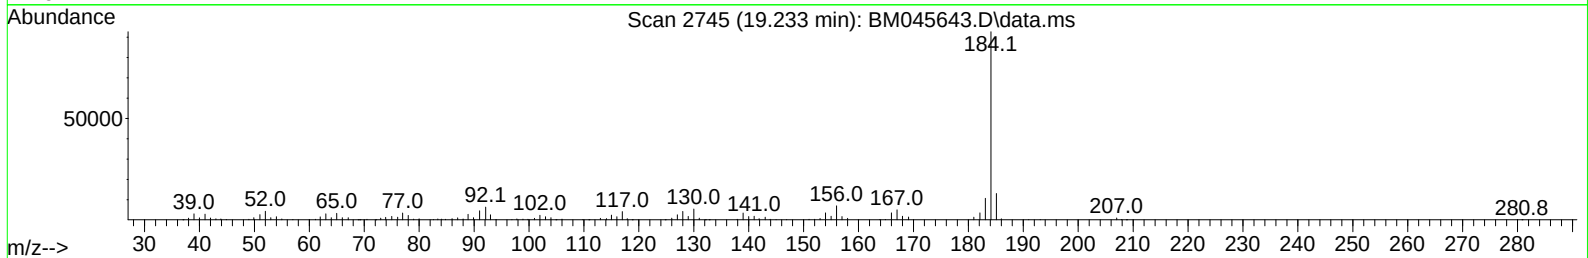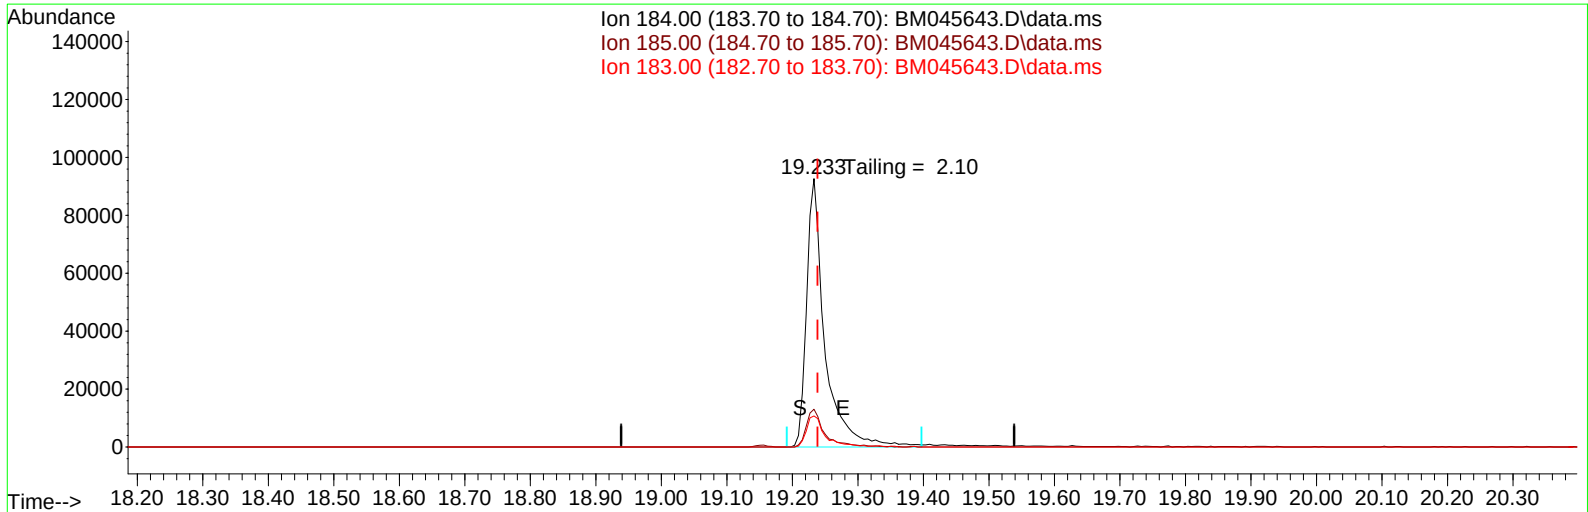

TIC: BM045643.D\data.ms

(77) Benzidine

19.233min (-0.006) 14711.34 ng

response 179365

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.08
183.00	11.70	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/30/2024	BNA_M	<u>BM045643.D</u>
Compound Name	Response	Retention Time
DDT	108703	20.456
DDD	2425	20.021
DDE	0	19.498
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2425	111128	2.18

Instrument :
BNA_M
ClientSampleId :
DFTPP