

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050115\
 Data File : BM001177.D
 Acq On : 02 May 2015 21:12
 Operator : TP/IZ
 Sample : G2058-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-10

Quant Time: May 04 01:52:56 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 04 01:38:30 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	18204	5.00	ng	0.00
6) Naphthalene-d8	10.31	136	68266	5.00	ng	0.00
12) Acenaphthene-d10	14.20	164	37392	5.00	ng	0.00
18) Phenanthrene-d10	16.94	188	90934	5.00	ng	0.00
24) Chrysene-d12	21.15	240	62287	5.00	ng	0.00
30) Perylene-d12	23.29	264	46259	5.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.13	112	222225	62.77	ng/uL	0.02
5) Phenol-d6	6.71	99	183183	41.99	ng/uL	0.00
7) Nitrobenzene-d5	8.69	82	430511	111.33	ng	0.00
13) 2,4,6-Tribromophenol	15.69	330	247121	132.78	ng/uL	0.00
14) 2-Fluorobiphenyl	12.81	172	1115143	90.18	ng	0.00
26) Terphenyl-d14	19.59	244	840759	97.90	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) n-Nitrosodimethylamine	3.27	42	96	0.04	ng	# 1
8) Nitrobenzene	8.69	77	1495	0.44	ng/uL#	37
9) Naphthalene	10.36	128	1453	0.10	ng	# 88
10) Hexachlorobutadiene	10.65	225	9	0.00	ng/uL#	1
11) 2-Methylnaphthalene	11.99	142	227	0.02	ng	# 84
15) Acenaphthylene	13.91	152	51	0.00	ng	# 67
16) Acenaphthene	14.18	154	232	0.02	ng	# 4
19) Hexachlorobenzene	15.97	284	363	0.07	ng	# 42
20) Pentachlorophenol	16.61	266	14	0.23	ng	# 59
21) Phenanthrene	16.98	178	339	0.01	ng	# 81
22) Anthracene	17.08	178	244	0.01	ng	# 76
23) Fluoranthene	19.01	202	135	0.01	ng	# 34
25) Pyrene	19.38	202	134	0.01	ng	# 71
27) Benzo(a)anthracene	21.14	228	312	0.02	ng	# 65
28) Chrysene	21.14	228	312	0.02	ng	# 68
29) Indeno(1,2,3-cd)pyrene	25.44	276	51	0.00	ng	# 47
31) Benzo(b)fluoranthene	22.66	252	57	0.00	ng	# 1
32) Benzo(k)fluoranthene	22.66	252	57	0.00	ng	# 1
33) Benzo(a)pyrene	23.20	252	44	0.00	ng	# 1
34) Dibenzo(a,h)anthracene	25.45	278	41	0.00	ng	# 1
35) Benzo(g,h,i)perylene	26.09	276	41	0.00	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050115\
Data File : BM001177.D
Acq On : 02 May 2015 21:12
Operator : TP/IZ
Sample : G2058-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-10

Quant Time: May 04 01:52:56 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM050115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 04 01:38:30 2015
Response via : Initial Calibration

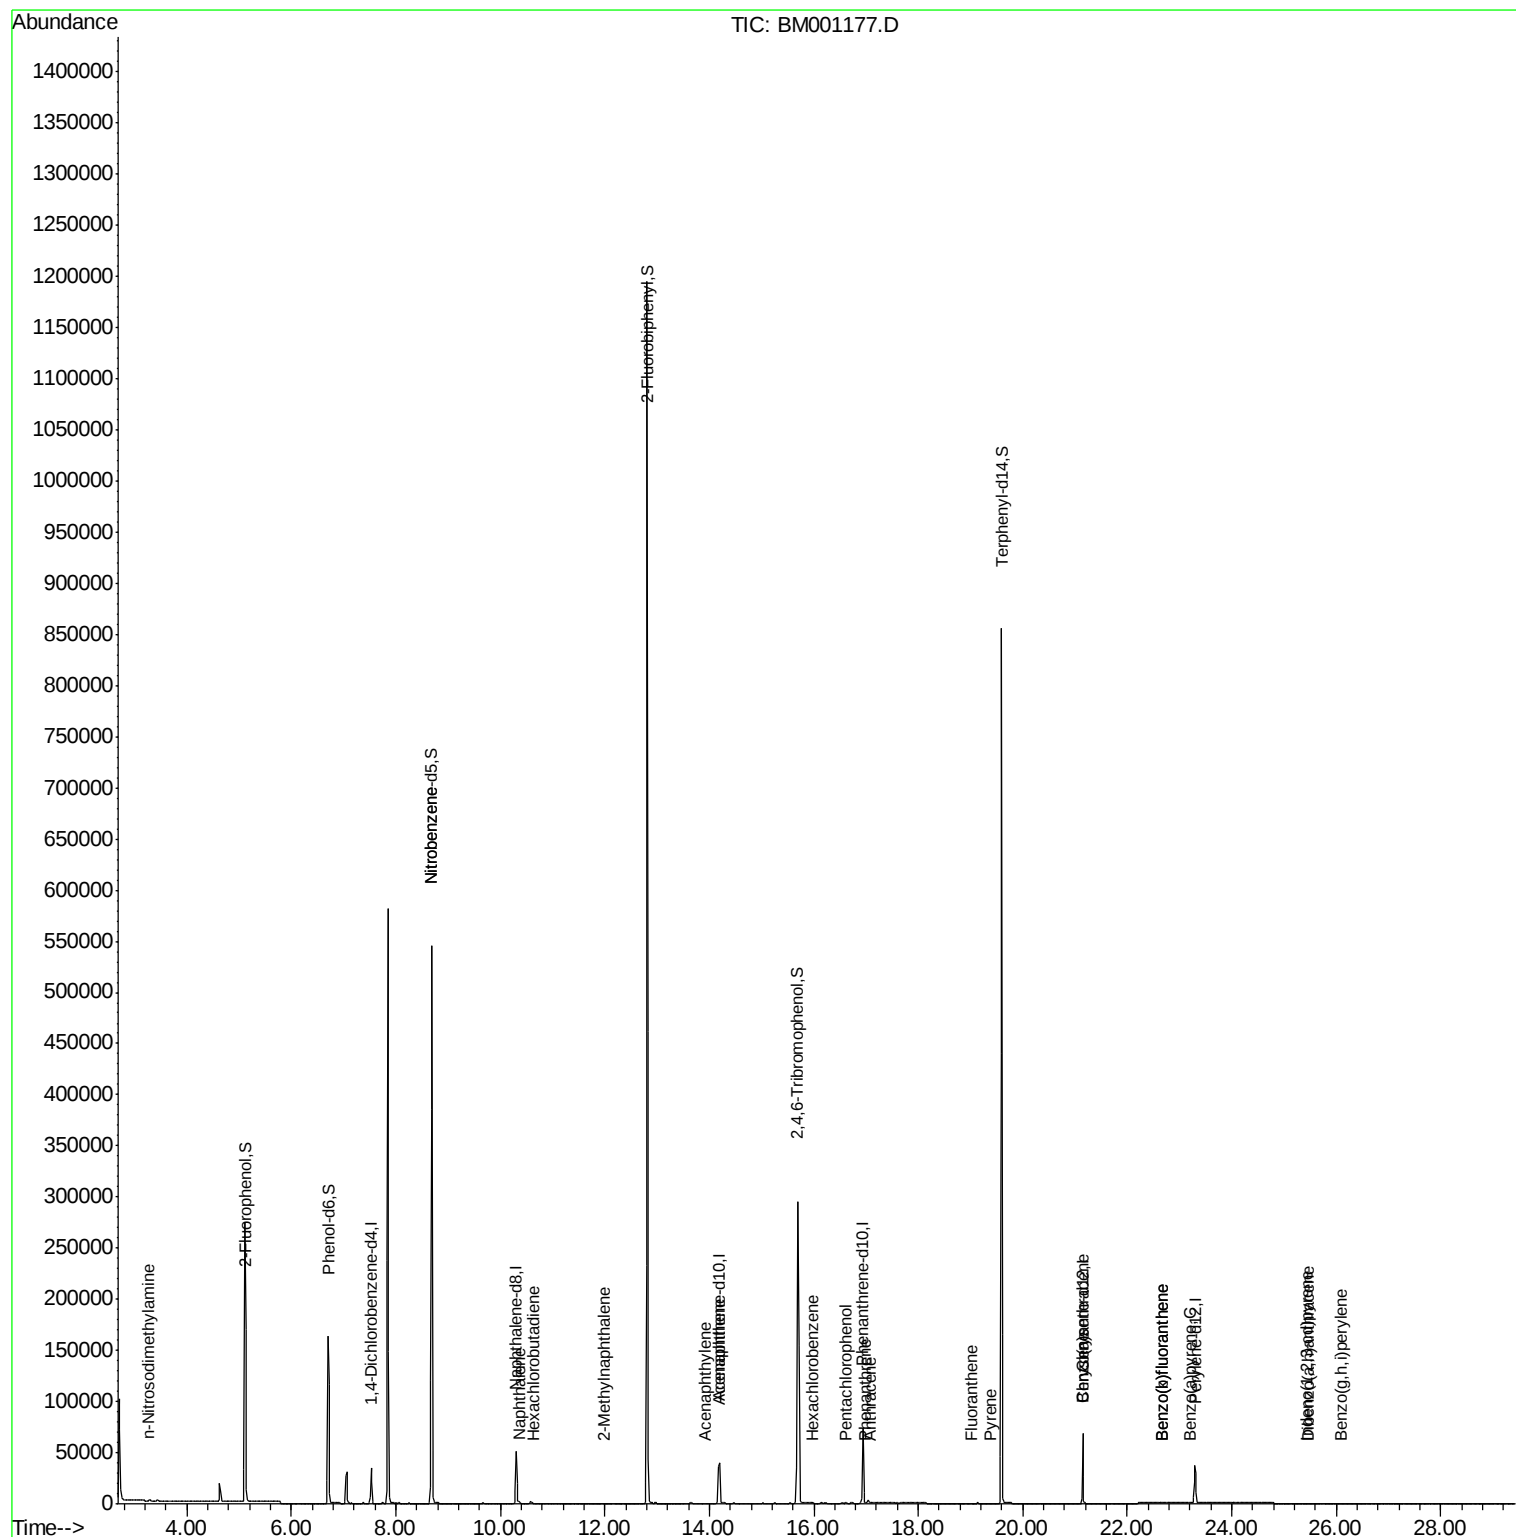




#1




1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.52 min Scan# 314
Delta R.T. -0.00 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Instrument :
BNA_M
ClientSampleId :
MW-10

Tgt Ion: 152 Resp: 18204
Ion Ratio Lower Upper
152 100
150 170.3 140.1 210.1
115 67.5 57.8 86.6

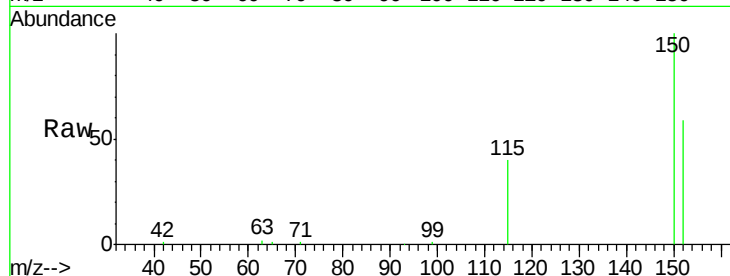


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

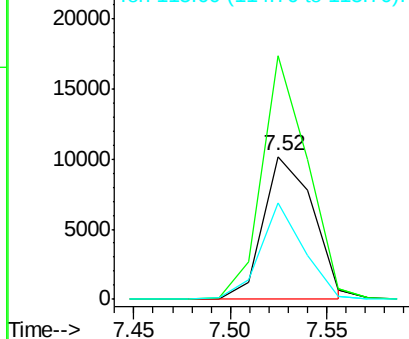



#3


n-Nitrosodimethylamine
Concen: 0.04 ng
RT: 3.27 min Scan# 39
Delta R.T. -0.06 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Tgt Ion: 42 Resp: 96
Ion Ratio Lower Upper
42 100
74 0.0 72.0 108.0#
44 127.1 3.7 5.5#



Abundance Ion 42.00 (41.70 to 42.70): BM0
Ion 74.00 (73.70 to 74.70): BM0
Ion 44.00 (43.70 to 44.70): BM0

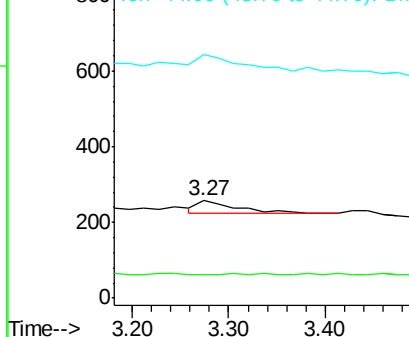



#4

2-Fluorophenol

Concen: 62.77 ng/uL

RT: 5.13 min Scan# 159

Delta R.T. 0.02 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampled :

MW-10


Tgt Ion: 112 Resp: 222225

Ion Ratio Lower Upper

112 100

64 63.9 52.6 79.0




63 35.2 29.5 44.3

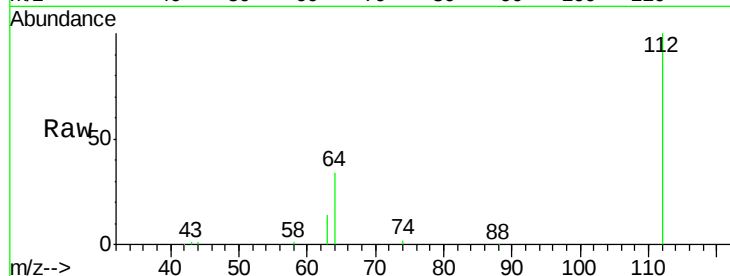

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): B

Ion 63.00 (62.70 to 63.70): B

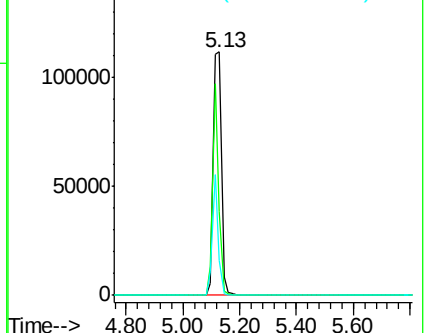

#5

Phenol-d6

Concen: 41.99 ng/uL

RT: 6.71 min Scan# 261

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion: 99 Resp: 183183

Ion Ratio Lower Upper

99 100

42 23.5 20.9 31.3



71 34.8 28.5 42.7




Abundance Ion 99.00 (98.70 to 99.70): B

Ion 42.00 (41.70 to 42.70): B

Ion 71.00 (70.70 to 71.70): B

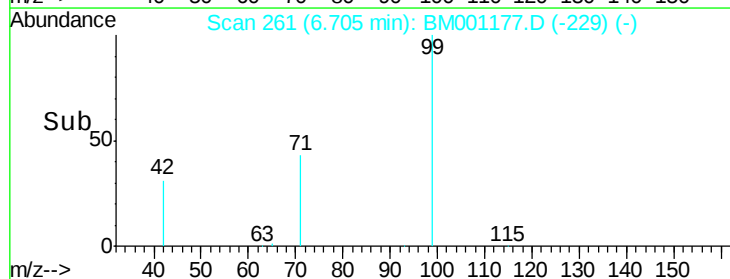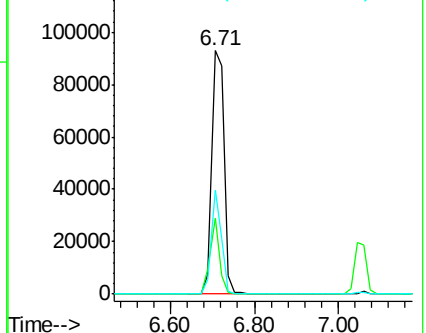



#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.31 min Scan# 532

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10





Tgt Ion: 136 Resp: 68266

Ion Ratio Lower Upper

136 100

137 10.6 8.2 12.4

54 10.1 9.0 13.4

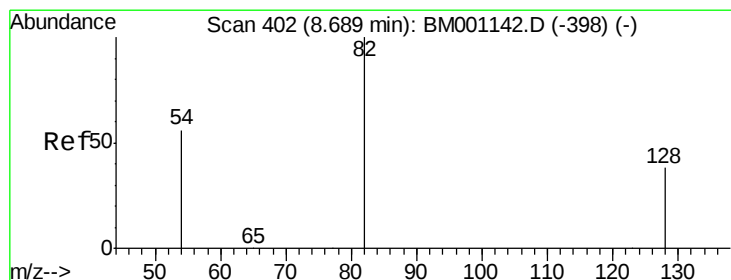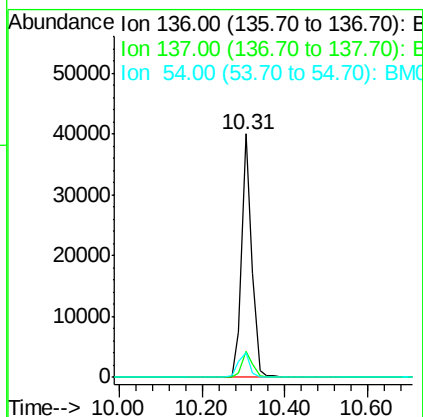

#7

Nitrobenzene-d5

Concen: 111.33 ng

RT: 8.69 min Scan# 402

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12




Tgt Ion: 82 Resp: 430511


Ion Ratio Lower Upper

82 100

128 42.2 31.9 47.9

54 53.9 46.2 69.2

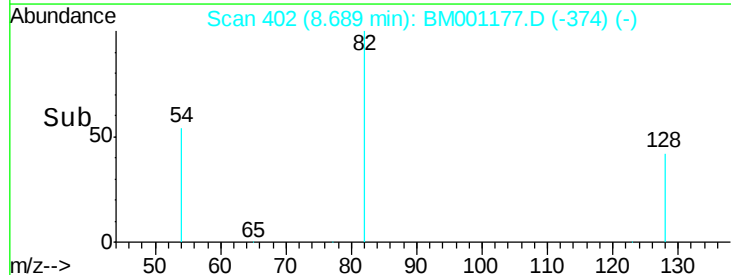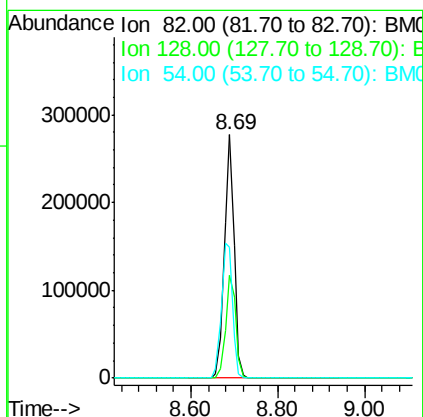

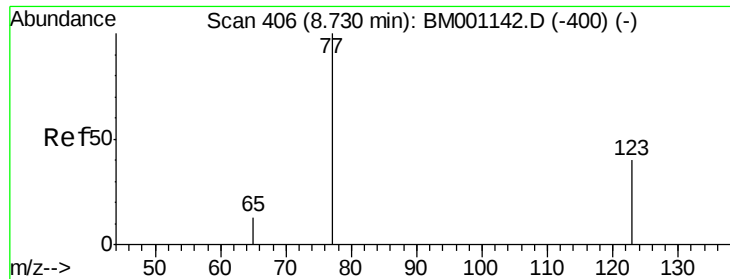

#8

Nitrobenzene

Concen: 0.44 ng/uL

RT: 8.69 min Scan# 402

Delta R.T. -0.04 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10


Tgt Ion: 77 Resp: 1495

Ion Ratio Lower Upper

77 100

123 0.0 31.0 46.6#




65 36.9 10.6 15.8#

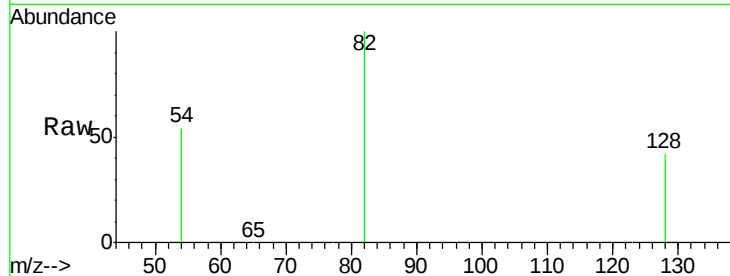

Abundance Ion 77.00 (76.70 to 77.70): BM001142.D (-400) (-)

Ion 123.00 (122.70 to 123.70): BM001142.D (-400) (-)

Ion 65.00 (64.70 to 65.70): BM001142.D (-400) (-)

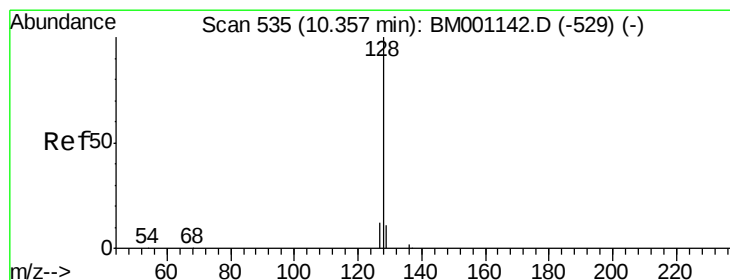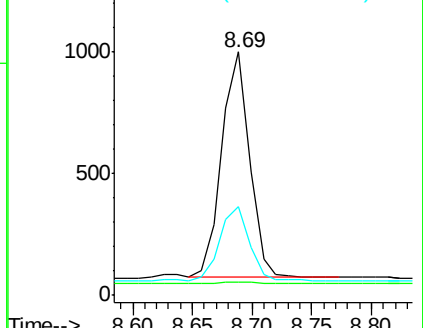

#9

Naphthalene

Concen: 0.10 ng

RT: 10.36 min Scan# 535

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion: 128 Resp: 1453

Ion Ratio Lower Upper

128 100

129 16.0 9.0 13.6#



127 16.9 10.0 15.0#




Abundance Ion 128.00 (127.70 to 128.70): BM001142.D (-529) (-)

Ion 129.00 (128.70 to 129.70): BM001142.D (-529) (-)

Ion 127.00 (126.70 to 127.70): BM001142.D (-529) (-)




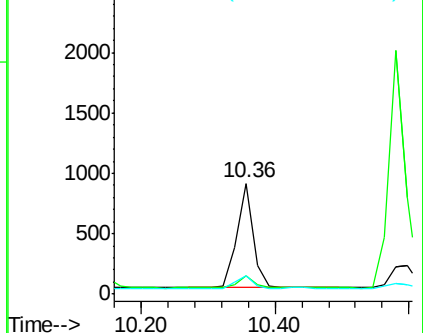




#10
Hexachlorobutadiene
Concen: 0.00 ng/uL
RT: 10.65 min Scan# 552
Delta R.T. -0.00 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12




Instrument :
BNA_M
ClientSampleId :
MW-10


Tgt Ion: 225 Resp: 9
Ion Ratio Lower Upper
225 100
223 222.2 50.8 76.2#
227 111.1 51.0 76.4#

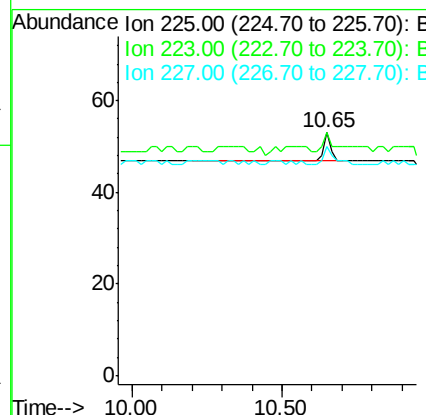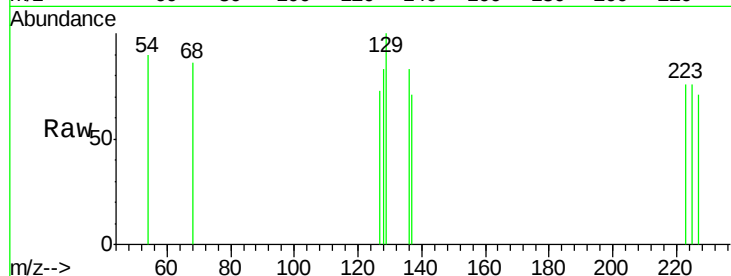

#11
2-Methylnaphthalene
Concen: 0.02 ng
RT: 11.99 min Scan# 661
Delta R.T. 0.01 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Tgt Ion: 142 Resp: 227
Ion Ratio Lower Upper
142 100
141 86.0 65.1 97.7
115 56.7 25.1 37.7#

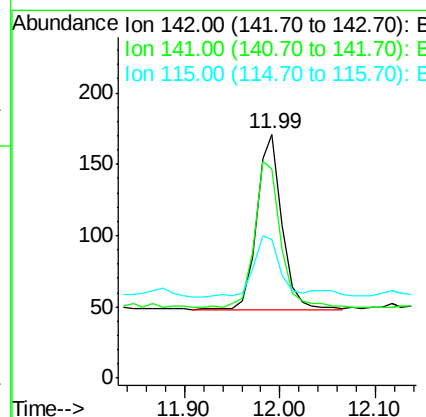



#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.20 min Scan# 838

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10


Tgt Ion:164 Resp: 37392

Ion Ratio Lower Upper

164 100

162 90.8 72.7 109.1




160 35.7 28.7 43.1

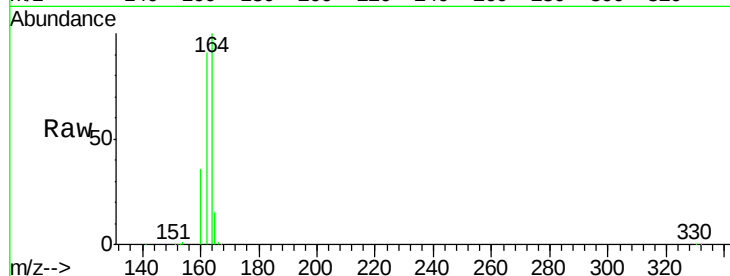

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

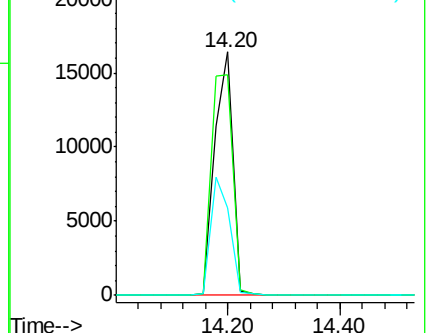

#13

2,4,6-Tribromophenol

Concen: 132.78 ng/uL

RT: 15.69 min Scan# 905

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion:330 Resp: 247121

Ion Ratio Lower Upper

330 100

332 97.8 74.5 111.7



141 44.9 21.0 31.4#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

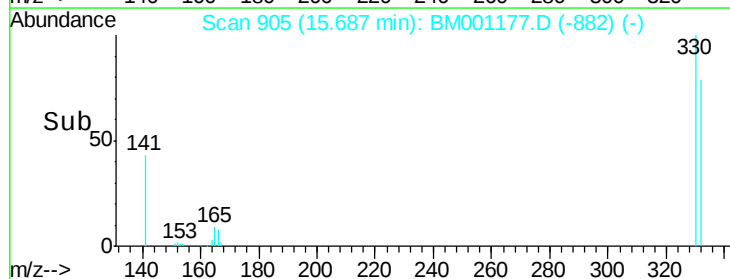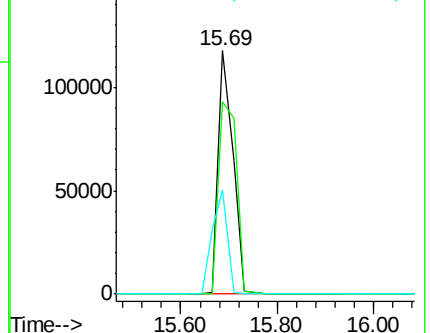


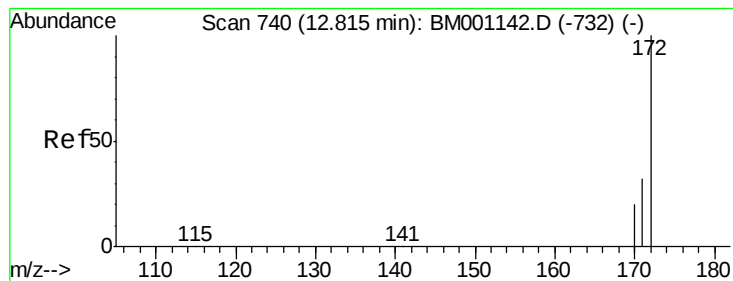




#14
2-Fluorobiphenyl
Concen: 90.18 ng
RT: 12.81 min Scan# 740
Delta R.T. -0.00 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Instrument :
BNA_M
ClientSampleId :
MW-10

Tgt Ion:172 Resp: 1115143
Ion Ratio Lower Upper
172 100
171 32.9 25.8 38.6
170 20.3 16.1 24.1

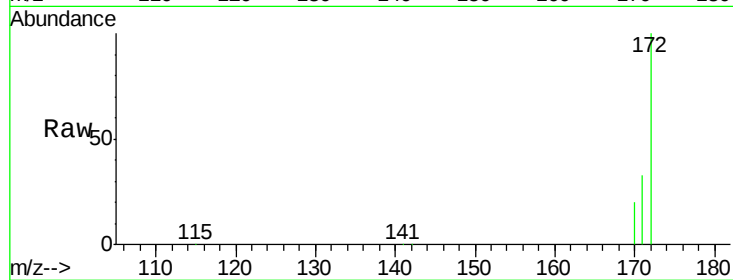


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

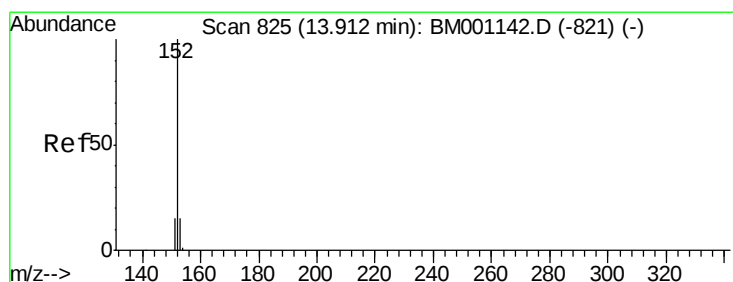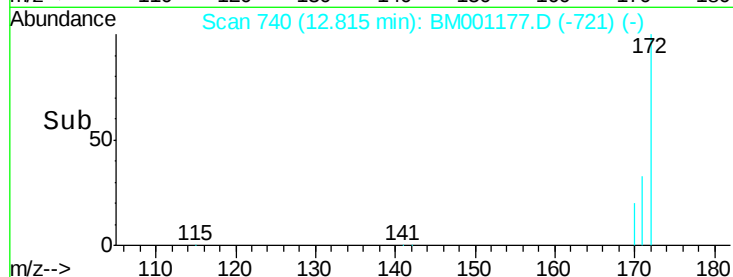
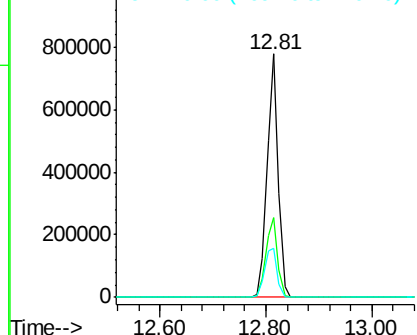



#15
Acenaphthylene
Concen: 0.00 ng
RT: 13.91 min Scan# 825
Delta R.T. 0.02 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Tgt Ion:152 Resp: 51
Ion Ratio Lower Upper
152 100
151 0.0 0.0 0.0
153 0.0 10.3 15.5#

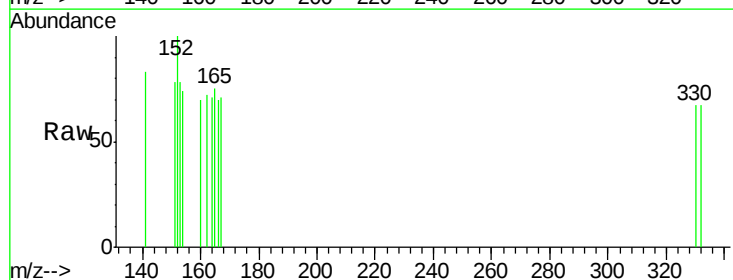

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

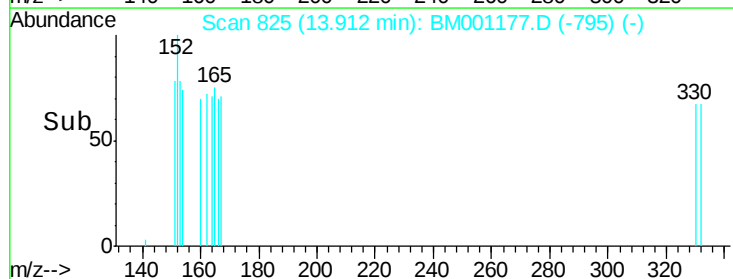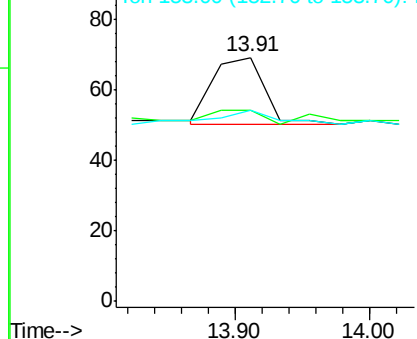



#16

Acenaphthene

Concen: 0.02 ng

RT: 14.18 min Scan# 837

Delta R.T. -0.07 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10


Tgt Ion:154 Resp: 232

Ion Ratio Lower Upper

154 100

153 0.0 90.6 136.0#




152 0.0 45.0 67.4#

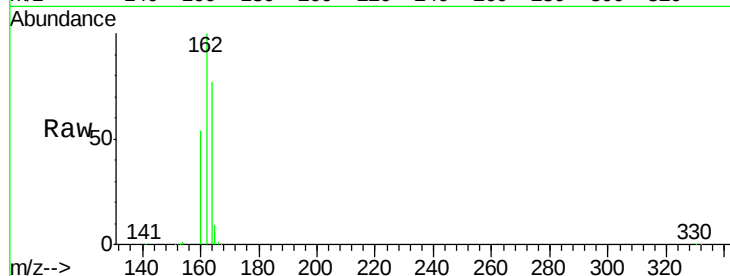

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

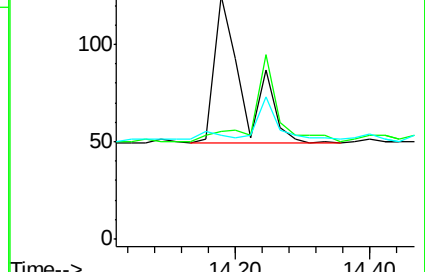

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.94 min Scan# 965

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion:188 Resp: 90934

Ion Ratio Lower Upper

188 100

94 10.1 9.3 13.9



80 10.3 9.8 14.6




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

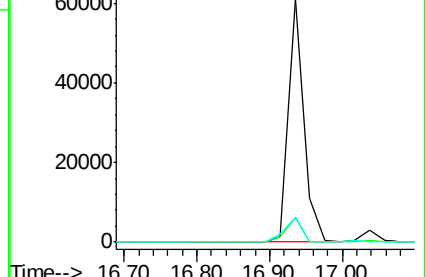







#19
Hexachlorobenzene
Concen: 0.07 ng
RT: 15.97 min Scan# 918
Delta R.T. -0.29 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Instrument :
BNA_M
ClientSampled :
MW-10

Tgt Ion: 284 Resp: 363
Ion Ratio Lower Upper
284 100
142 0.0 0.0 0.0
249 0.0 26.5 39.7#




Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E


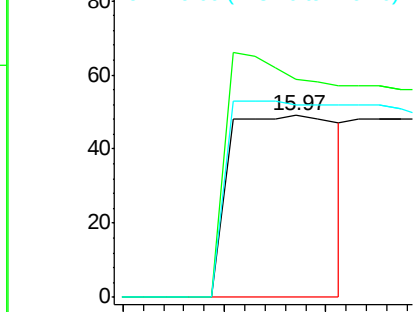



#20
Pentachlorophenol
Concen: 0.23 ng
RT: 16.61 min Scan# 949
Delta R.T. -0.00 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Tgt Ion: 266 Resp: 14
Ion Ratio Lower Upper
266 100
268 100.0 52.6 79.0#
264 94.4 51.0 76.4#



Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

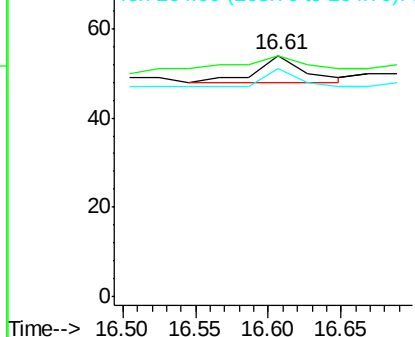

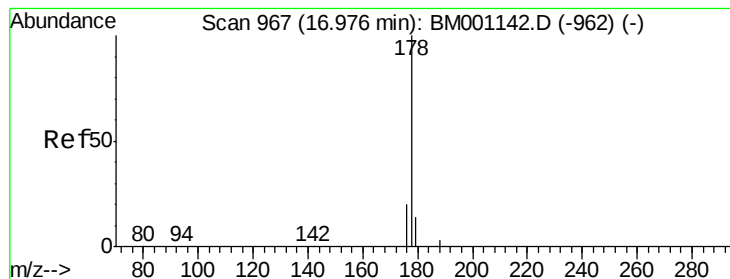

#21

Phenanthrene

Concen: 0.01 ng

RT: 16.98 min Scan# 967

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10


Tgt Ion:178 Resp: 339

Ion Ratio Lower Upper

178 100

176 21.8 15.5 23.3




179 0.0 12.0 18.0#



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

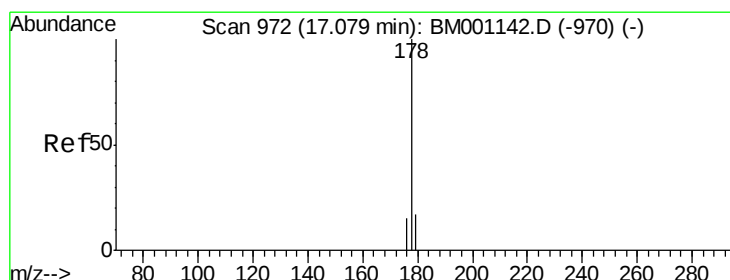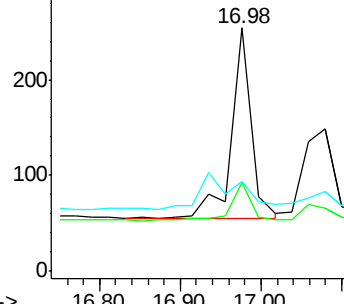

#22

Anthracene

Concen: 0.01 ng

RT: 17.08 min Scan# 972

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion:178 Resp: 244

Ion Ratio Lower Upper

178 100

176 0.0 14.3 21.5#



179 13.5 12.2 18.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

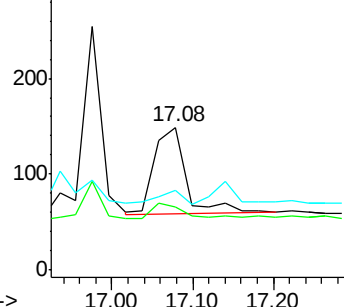



#23

Fluoranthene

Concen: 0.01 ng

RT: 19.01 min Scan# 1095

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10


Tgt Ion:202 Resp: 135

Ion Ratio Lower Upper

202 100

101 67.4 9.3 13.9#




203 22.2 13.7 20.5#



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

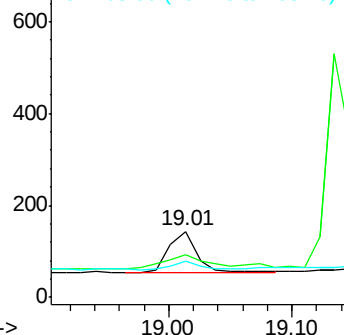

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.15 min Scan# 1279

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion:240 Resp: 62287

Ion Ratio Lower Upper

240 100

120 9.1 9.2 13.8#



236 26.5 22.4 33.6




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

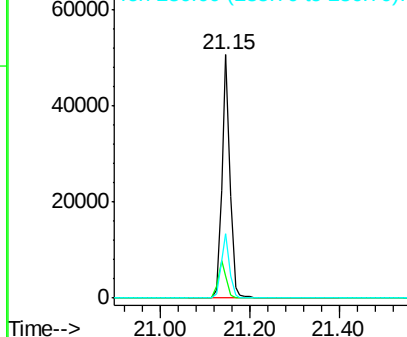

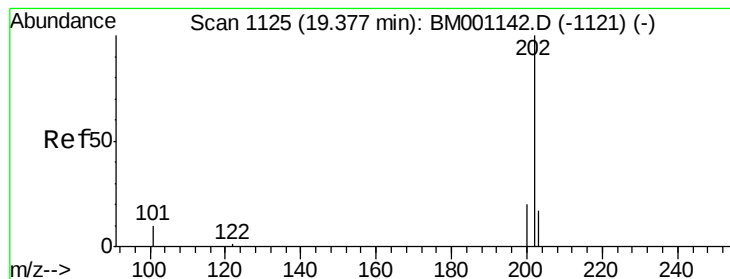

#25

Pyrene

Concen: 0.01 ng

RT: 19.38 min Scan# 1125

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10


Tgt Ion: 202 Resp: 134

Ion Ratio Lower Upper

202 100

200 0.0 16.4 24.6#


203 22.4 13.8 20.6#





Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

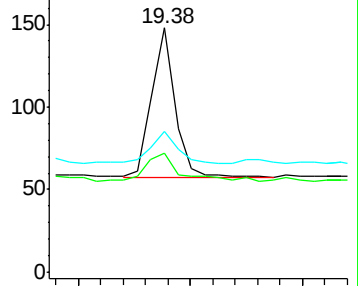

Time-->

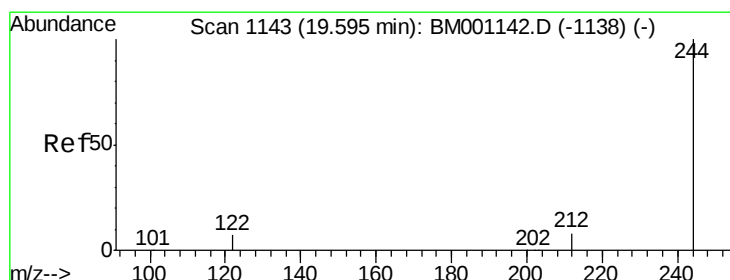

#26

Terphenyl-d14

Concen: 97.90 ng

RT: 19.59 min Scan# 1143

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion: 244 Resp: 840759

Ion Ratio Lower Upper

244 100

212 9.7 7.1 10.7


122 10.2 6.2 9.4#




Abundance Ion 244.00 (243.70 to 244.70): E


Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

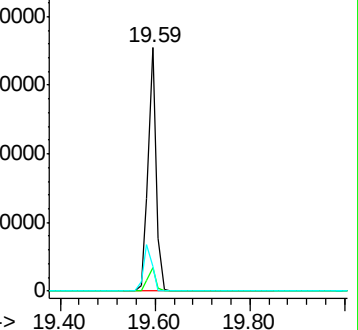

Time-->









#27
Benzo(a)anthracene
Concen: 0.02 ng
RT: 21.14 min Scan# 1278
Delta R.T. 0.01 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12




Instrument :
BNA_M
ClientSampleId :
MW-10


Tgt Ion:228 Resp: 312
Ion Ratio Lower Upper
228 100
226 35.9 22.8 34.2#
229 48.1 14.4 21.6#

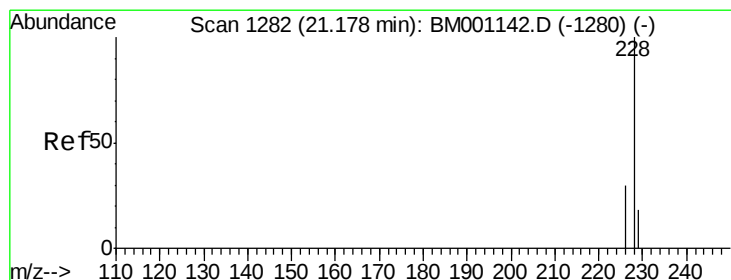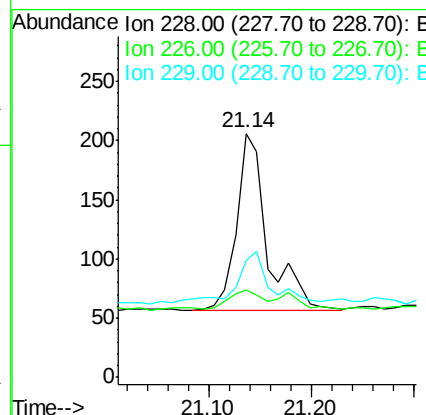

#28
Chrysene
Concen: 0.02 ng
RT: 21.14 min Scan# 1278
Delta R.T. -0.04 min
Lab File: BM001177.D
Acq: 02 May 2015 21:12

Tgt Ion:228 Resp: 312
Ion Ratio Lower Upper
228 100
226 35.9 24.4 36.6
229 48.1 14.3 21.5#

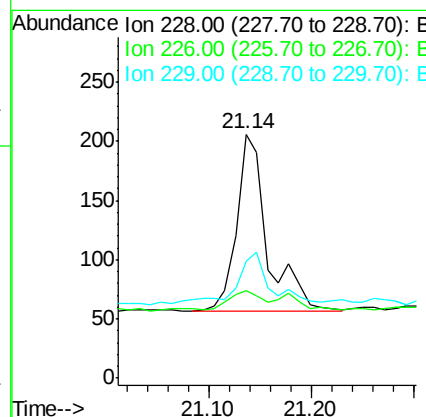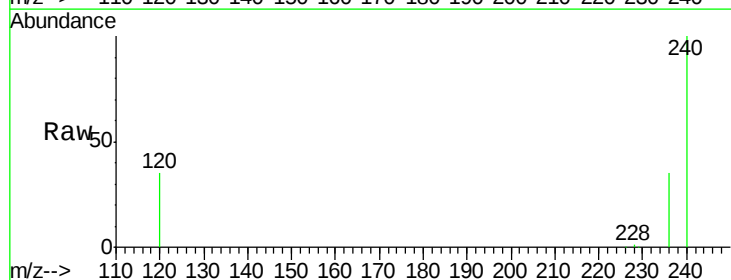



#29

Indeno(1,2,3-cd)pyrene

Concen: 0.00 ng

RT: 25.44 min Scan# 1691

Delta R.T. 0.01 min

Lab File: BM001177.D


Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10






Tgt Ion: 276 Resp: 51

Ion Ratio Lower Upper

276 100

138 0.0 24.2 36.4#

277 0.0 19.8 29.6#

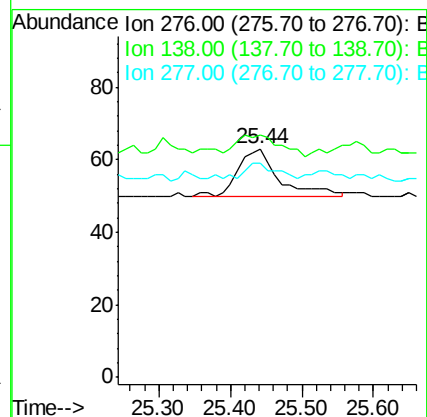

#30

Perylene-d12

Concen: 5.00 ng

RT: 23.29 min Scan# 1485

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12




Tgt Ion: 264 Resp: 46259


Ion Ratio Lower Upper

264 100

260 26.0 18.9 28.3

265 21.2 18.1 27.1

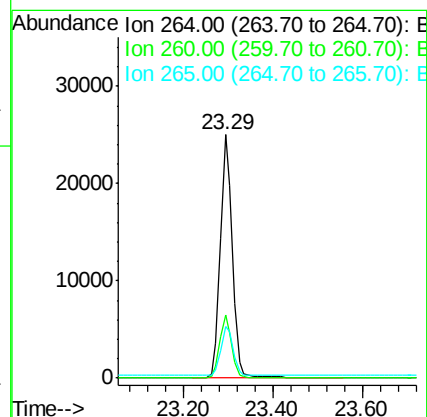



#31

Benzo(b)fluoranthene

Concen: 0.00 ng

RT: 22.66 min Scan# 1424

Delta R.T. 0.01 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10


Tgt Ion:252 Resp: 57

Ion Ratio Lower Upper




252 100

253 169.7 19.0 28.4#

125 100.8 9.1 13.7#

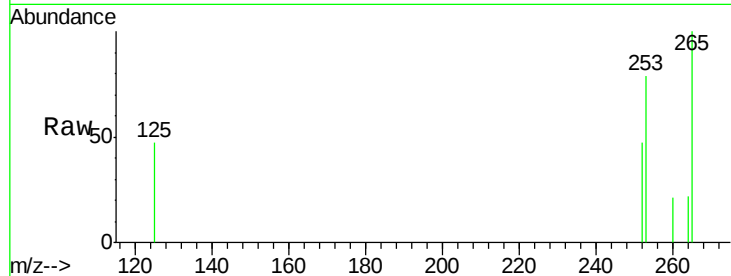

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

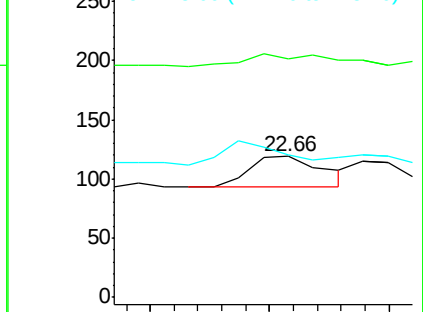

#32

Benzo(k)fluoranthene

Concen: 0.00 ng

RT: 22.66 min Scan# 1424

Delta R.T. -0.03 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12


Tgt Ion:252 Resp: 57

Ion Ratio Lower Upper



252 100


253 169.7 19.1 28.7#

125 100.8 9.3 13.9#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

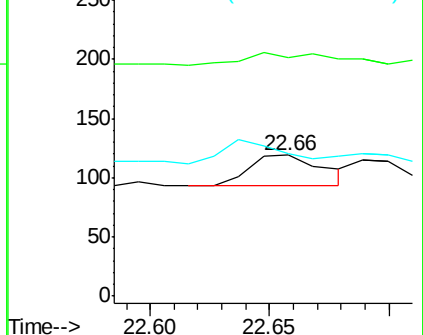



#33

Benzo(a)pyrene

Concen: 0.00 ng

RT: 23.20 min Scan# 1476

Delta R.T. -0.00 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Instrument :


BNA_M

ClientSampleId :

MW-10

Tgt Ion: 252 Resp: 44




Ion	Ratio	Lower	Upper
252	100		
253	177.9	18.2	27.2#
125	101.8	10.6	16.0#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

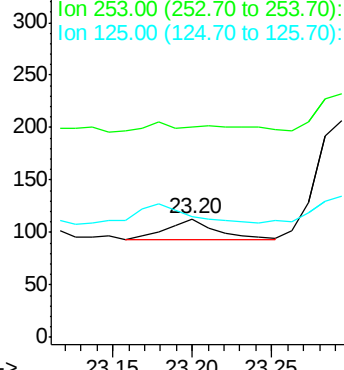

#34

Dibenzo(a,h)anthracene

Concen: 0.00 ng

RT: 25.45 min Scan# 1692


Delta R.T. 0.01 min

Lab File: BM001177.D

Acq: 02 May 2015 21:12

Tgt Ion: 278 Resp: 41



Ion	Ratio	Lower	Upper
278	100		
139	116.4	15.5	23.3#
279	137.7	19.7	29.5#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

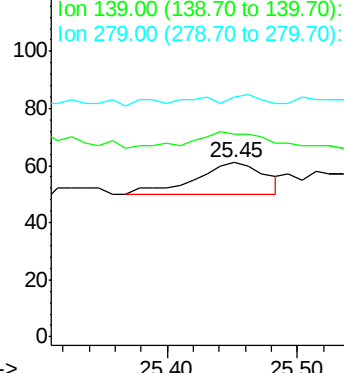



#35

Benzo(g,h,i)perylene

Concen: 0.00 ng

RT: 26.09 min Scan# 1753

Delta R.T. -0.00 min

Lab File: BM001177.D


Acq: 02 May 2015 21:12

Instrument :

BNA_M

ClientSampleId :

MW-10




Tgt Ion: 276 Resp: 41

Ion Ratio Lower Upper

276 100

277 92.1 19.0 28.4#

138 103.2 21.3 31.9#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

