


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050115\
Data File : BM001154.D
Acq On : 02 May 2015 05:42
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 30 19:07:47 2015

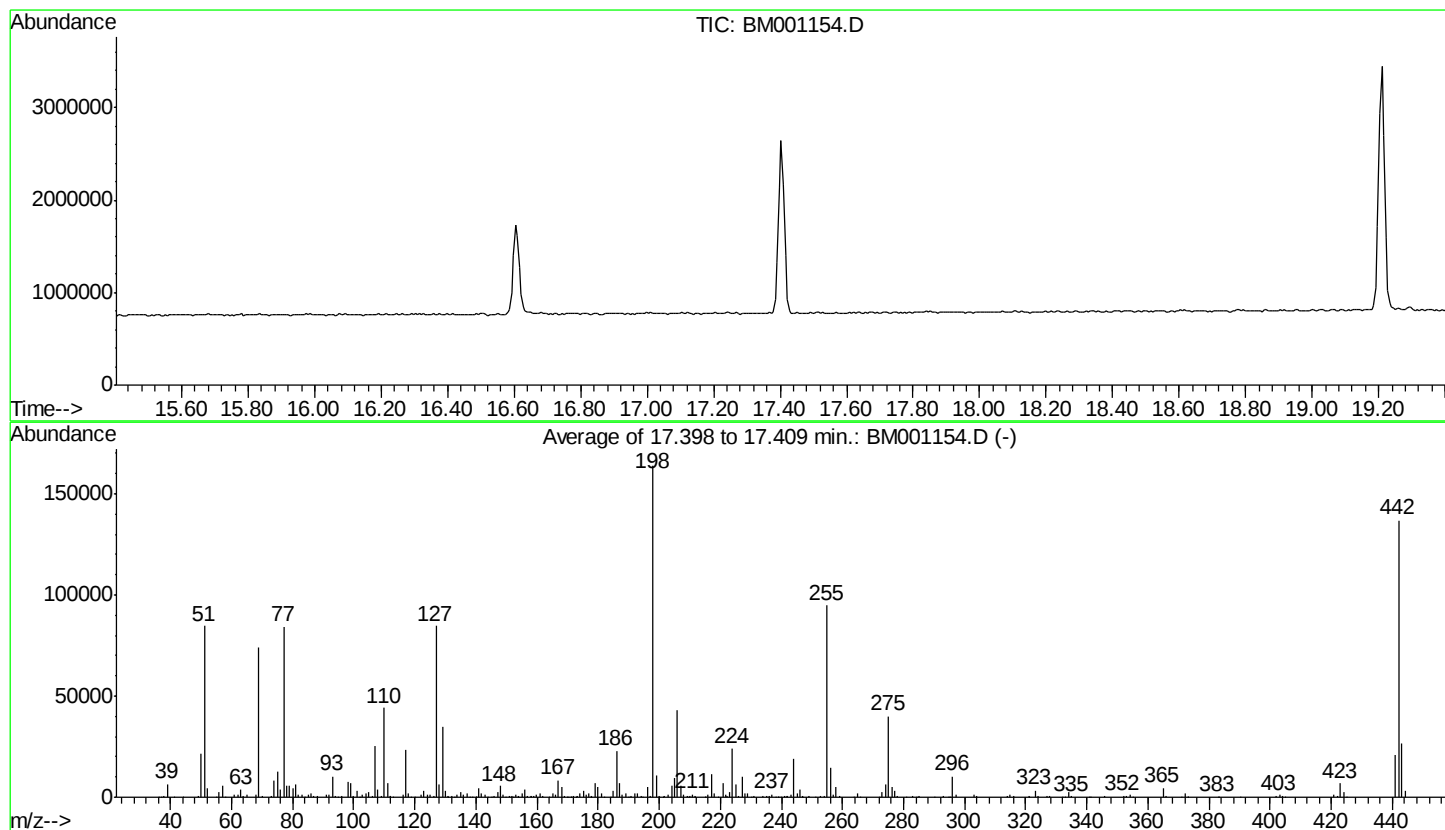

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	84546	PASS
68	69	0.00	2	1.8	1342	PASS
69	198	0.00	100	45.1	73912	PASS
70	69	0.00	2	0.5	379	PASS
127	198	10	80	51.7	84693	PASS
197	198	0.00	2	0.6	972	PASS
198	198	100	100	100.0	163904	PASS
199	198	5	9	6.6	10777	PASS
275	198	10	60	24.4	39914	PASS
365	198	1	100	2.8	4580	PASS
441	442	0.01	24	15.3	20975	PASS
442	198	50	100	83.4	136688	PASS
443	442	15	24	19.5	26680	PASS