


Data Path : Z:\HPCHEM1\BNA M\Data\BM050115\
 Data File : BM001154.D
 Acq On : 02 May 2015 05:42
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA M\METHODS\SIMPAH-BM050115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 18:16:53 2015

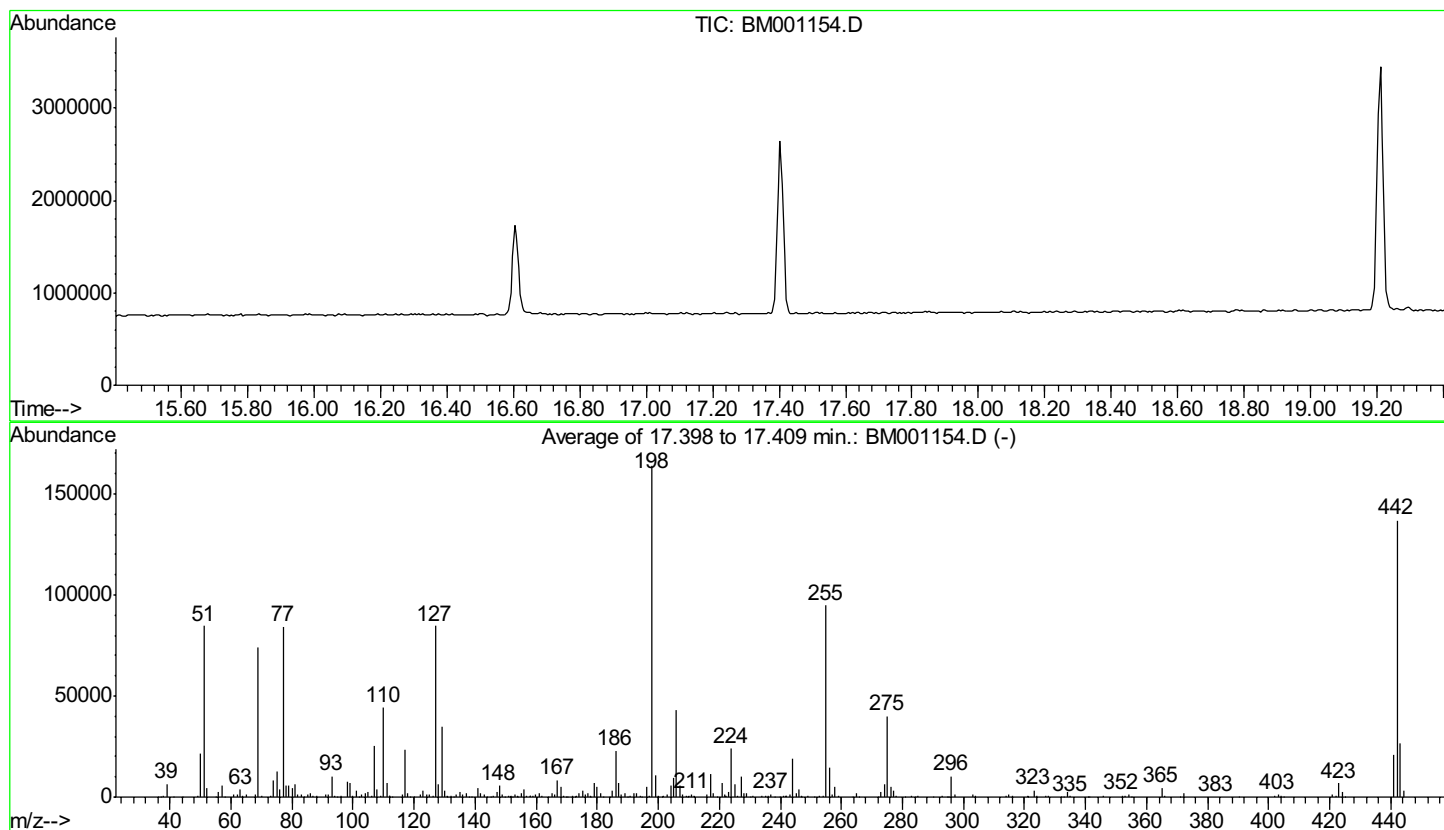

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	51.6	84546	PASS
68	69	0.00	2	1.8	1342	PASS
69	198	0.00	100	45.1	73912	PASS
70	69	0.00	2	0.5	379	PASS
127	198	10	80	51.7	84693	PASS
197	198	0.00	2	0.6	972	PASS
198	198	100	100	100.0	163904	PASS
199	198	5	9	6.6	10777	PASS
275	198	10	60	24.4	39914	PASS
365	198	1	100	2.8	4580	PASS
441	442	0.01	24	15.3	20975	PASS
442	198	50	100	83.4	136688	PASS
443	442	15	24	19.5	26680	PASS