


Data Path : Z:\HPCHEM1\BNA M\Data\BM050115\
 Data File : BM001171.D
 Acq On : 02 May 2015 17:01
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA M\METHODS\SIMPAH-BM050115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 18:16:53 2015

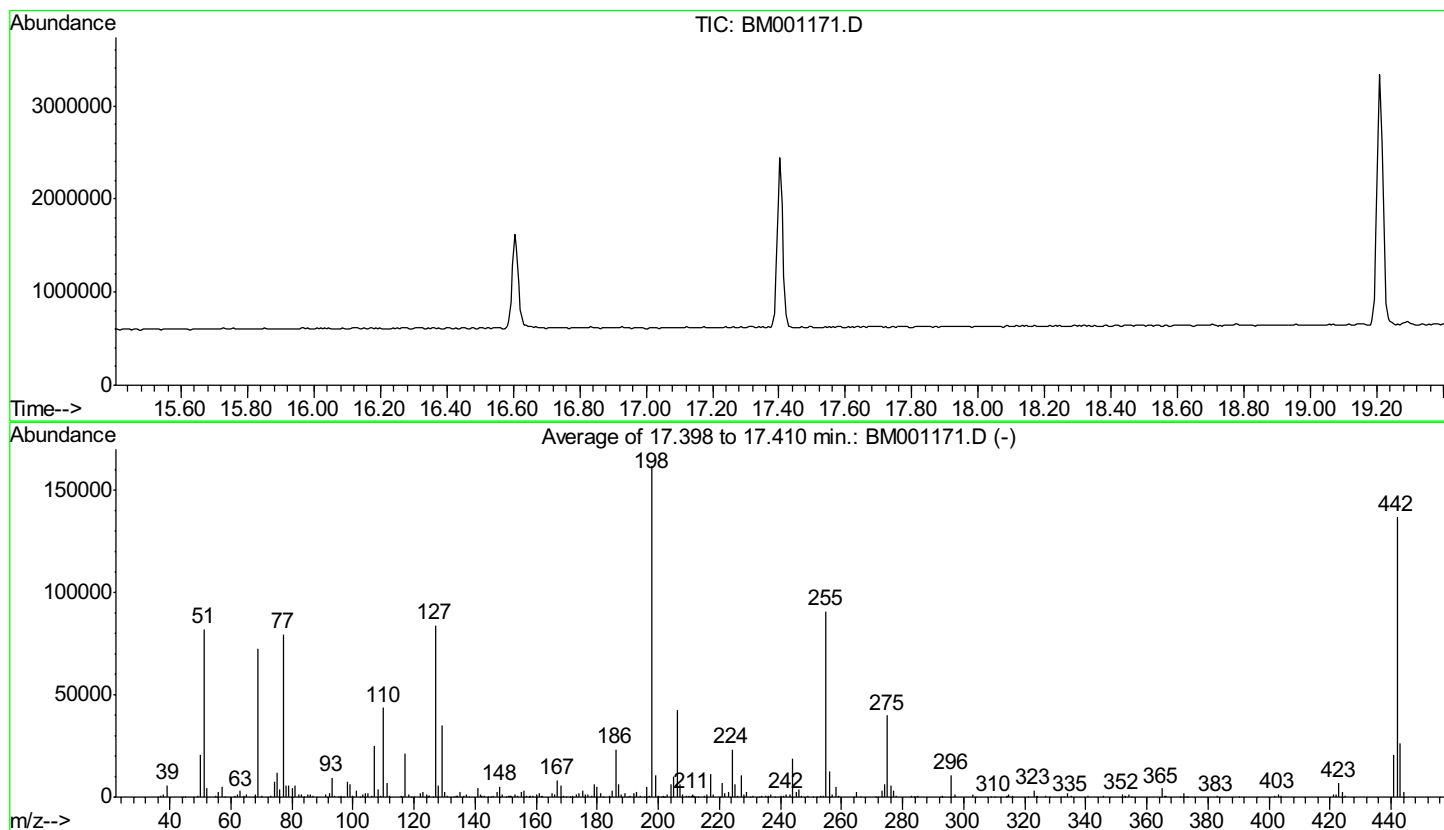

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	50.7	82064	PASS
68	69	0.00	2	1.7	1234	PASS
69	198	0.00	100	44.7	72330	PASS
70	69	0.00	2	0.6	423	PASS
127	198	10	80	51.8	83829	PASS
197	198	0.00	2	0.6	937	PASS
198	198	100	100	100.0	161877	PASS
199	198	5	9	6.6	10697	PASS
275	198	10	60	24.6	39856	PASS
365	198	1	100	2.6	4265	PASS
441	442	0.01	24	14.9	20362	PASS
442	198	50	100	84.7	137106	PASS
443	442	15	24	19.2	26360	PASS