

Data File : BM009833.D
Acq On : 01 May 2017 16:56
Operator : SJ/MA
Sample : PB98511BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK11

Quant Time: May 02 00:52:54 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 02 00:52:56 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	63940	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	295614	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	198800	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	529851	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	780005	20.00	ng/ul	0.00
83) Perylene-d12	23.72	264	852416	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	9040	6.51	ng/uL	0.00
5) Phenol-d5	6.99	99	197446	28.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	143938	30.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	132509	29.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	153555	28.36	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	73215	30.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	81874	32.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	139657	27.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	204675	33.55	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	570862	33.01	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	640981	30.73	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	87970	26.36	ng/ul	0.00
57) Fluorene-d10	15.46	176	484431	31.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	85164	22.78	ng/ul	0.00
70) Anthracene-d10	17.32	188	839606	30.86	ng/ul	0.00
76) Pyrene-d10	19.61	212	1065713	30.96	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1283261	30.95	ng/ul	0.00

Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.53	70	5642	1.02 ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM009833.D

Acq On : 01 May 2017 16:56

Operator : SJ/MA

Sample : PB98511BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

SBLK11


Quant Time: May 02 00:52:54 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue May 02 00:52:56 2017

Response via : Initial Calibration

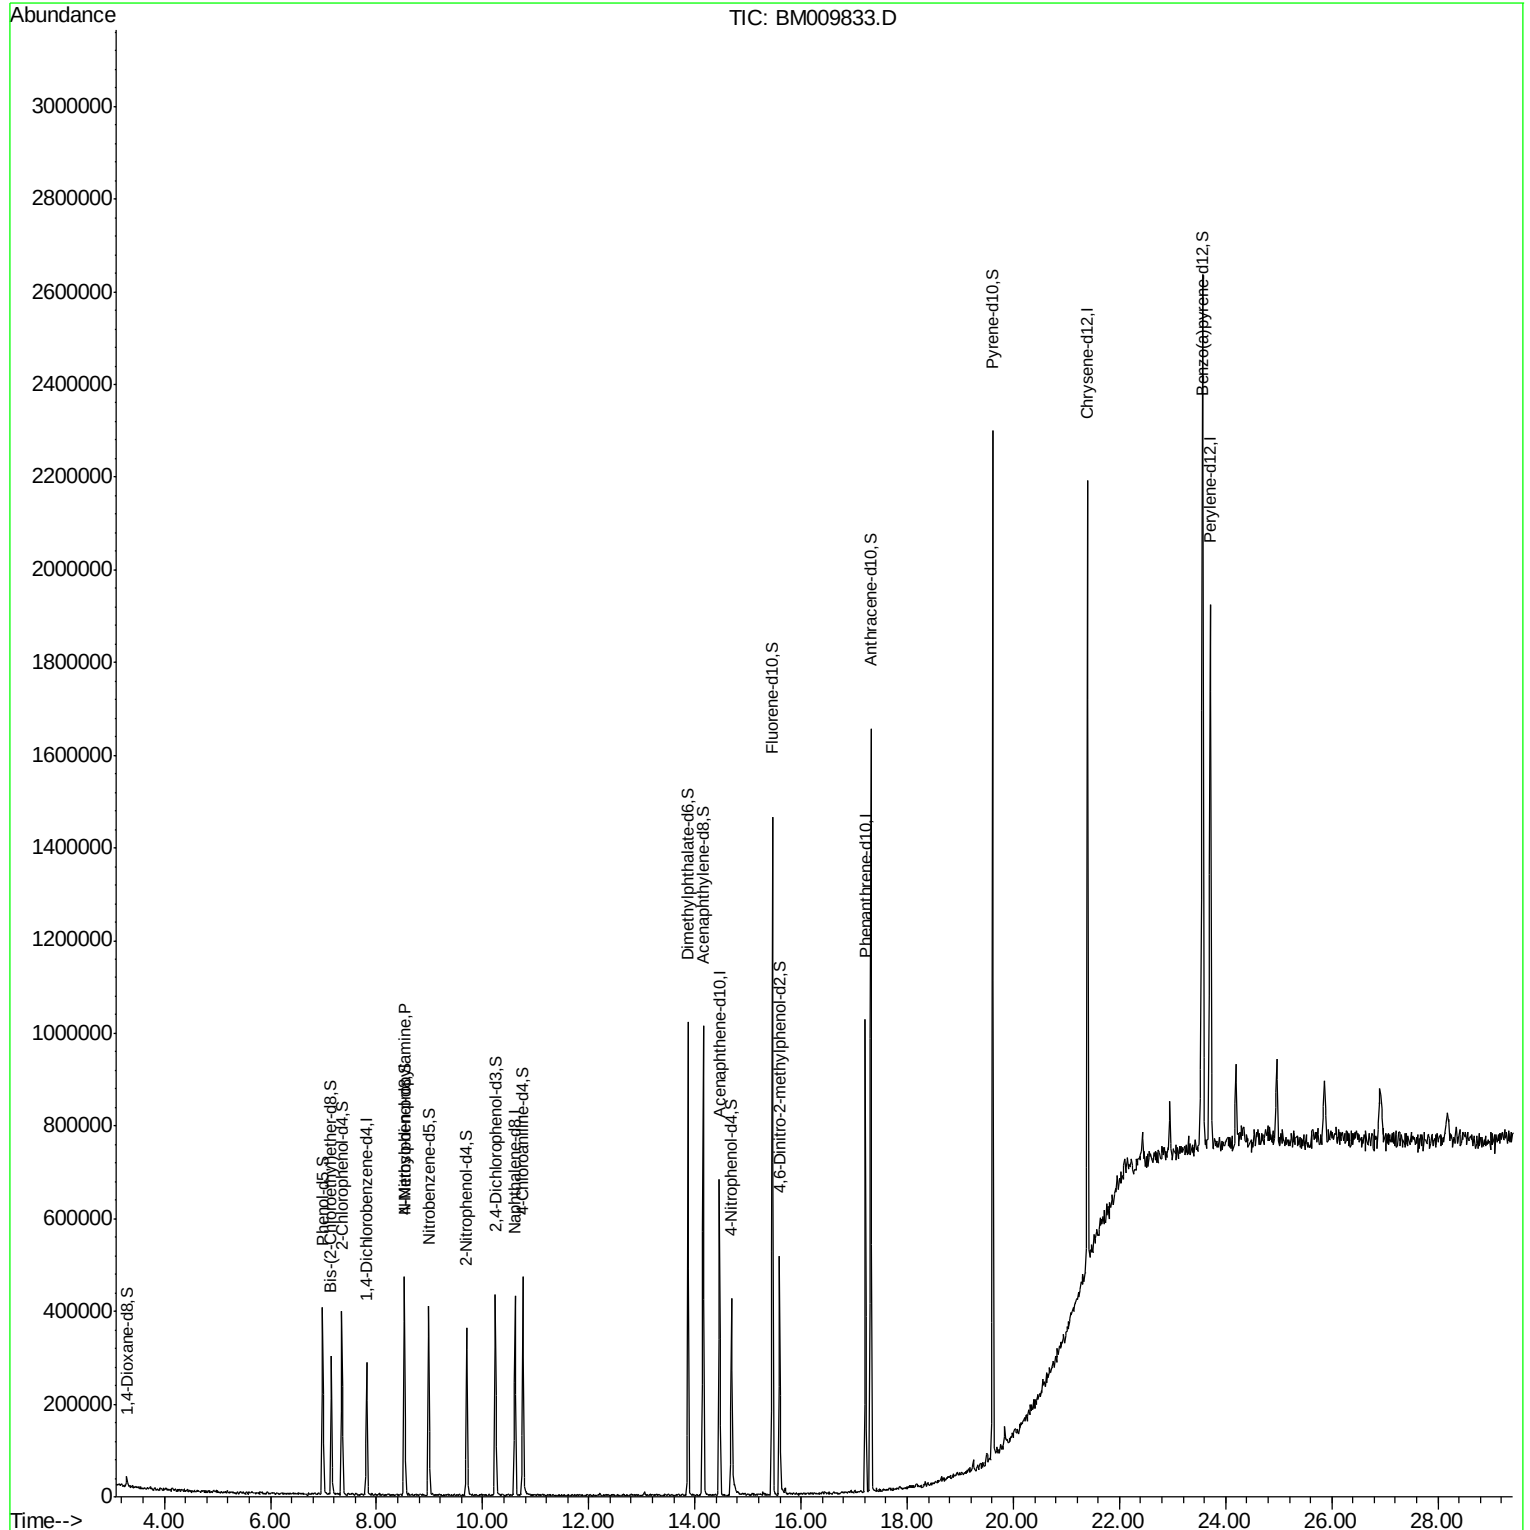

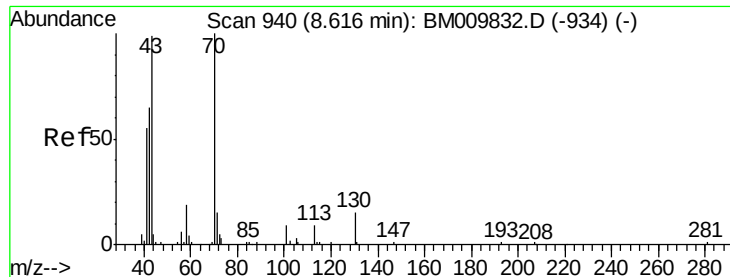

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.02 ng/ul
 RT: 8.53 min Scan# 925
 Delta R.T. -0.09 min
 Lab File: BM009833.D
 Acq: 01 May 2017 16:56

Instrument :
 BNA_M
 ClientSampleId :
 SBLK11

Tgt Ion:	70	Resp:	5642
Ion	Ratio	Lower	Upper
70	100		
42	313.1	64.2	96.2#
101	0.0	5.1	7.7#
130	0.0	8.3	12.5#

