

Data File : BM009836.D
Acq On : 01 May 2017 18:44
Operator : SJ/MA
Sample : I2848-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT06

Quant Time: May 02 00:53:31 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 02 00:52:56 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	73622	20.00	ng/ul	0.00
18) Naphthalene-d8	10.61	136	344038	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	242228	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	630635	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	917172	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1008762	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.29	96	8571	5.36	ng/uL	0.00
5) Phenol-d5	6.99	99	237975	29.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	175005	32.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	163542	32.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	188875	30.29	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	86647	30.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	98211	33.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	176317	29.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	249032	35.08	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	692800	32.88	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	811240	31.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	106546	26.21	ng/ul	0.00
57) Fluorene-d10	15.46	176	622935	32.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	98111	22.05	ng/ul	0.00
70) Anthracene-d10	17.31	188	1078388	33.30	ng/ul	0.00
76) Pyrene-d10	19.61	212	1374551	33.96	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1614886	32.92	ng/ul	0.00

Target Compounds				Qvalue		
6) Phenol	7.01	94	16437	1.99	ng/ul#	63
44) Dimethylphthalate	13.92	163	70118	3.36	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM009836.D

Acq On : 01 May 2017 18:44

Operator : SJ/MA

Sample : I2848-04

Misc :

ALS Vial : 6 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

JHT06


Quant Time: May 02 00:53:31 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue May 02 00:52:56 2017

Response via : Initial Calibration

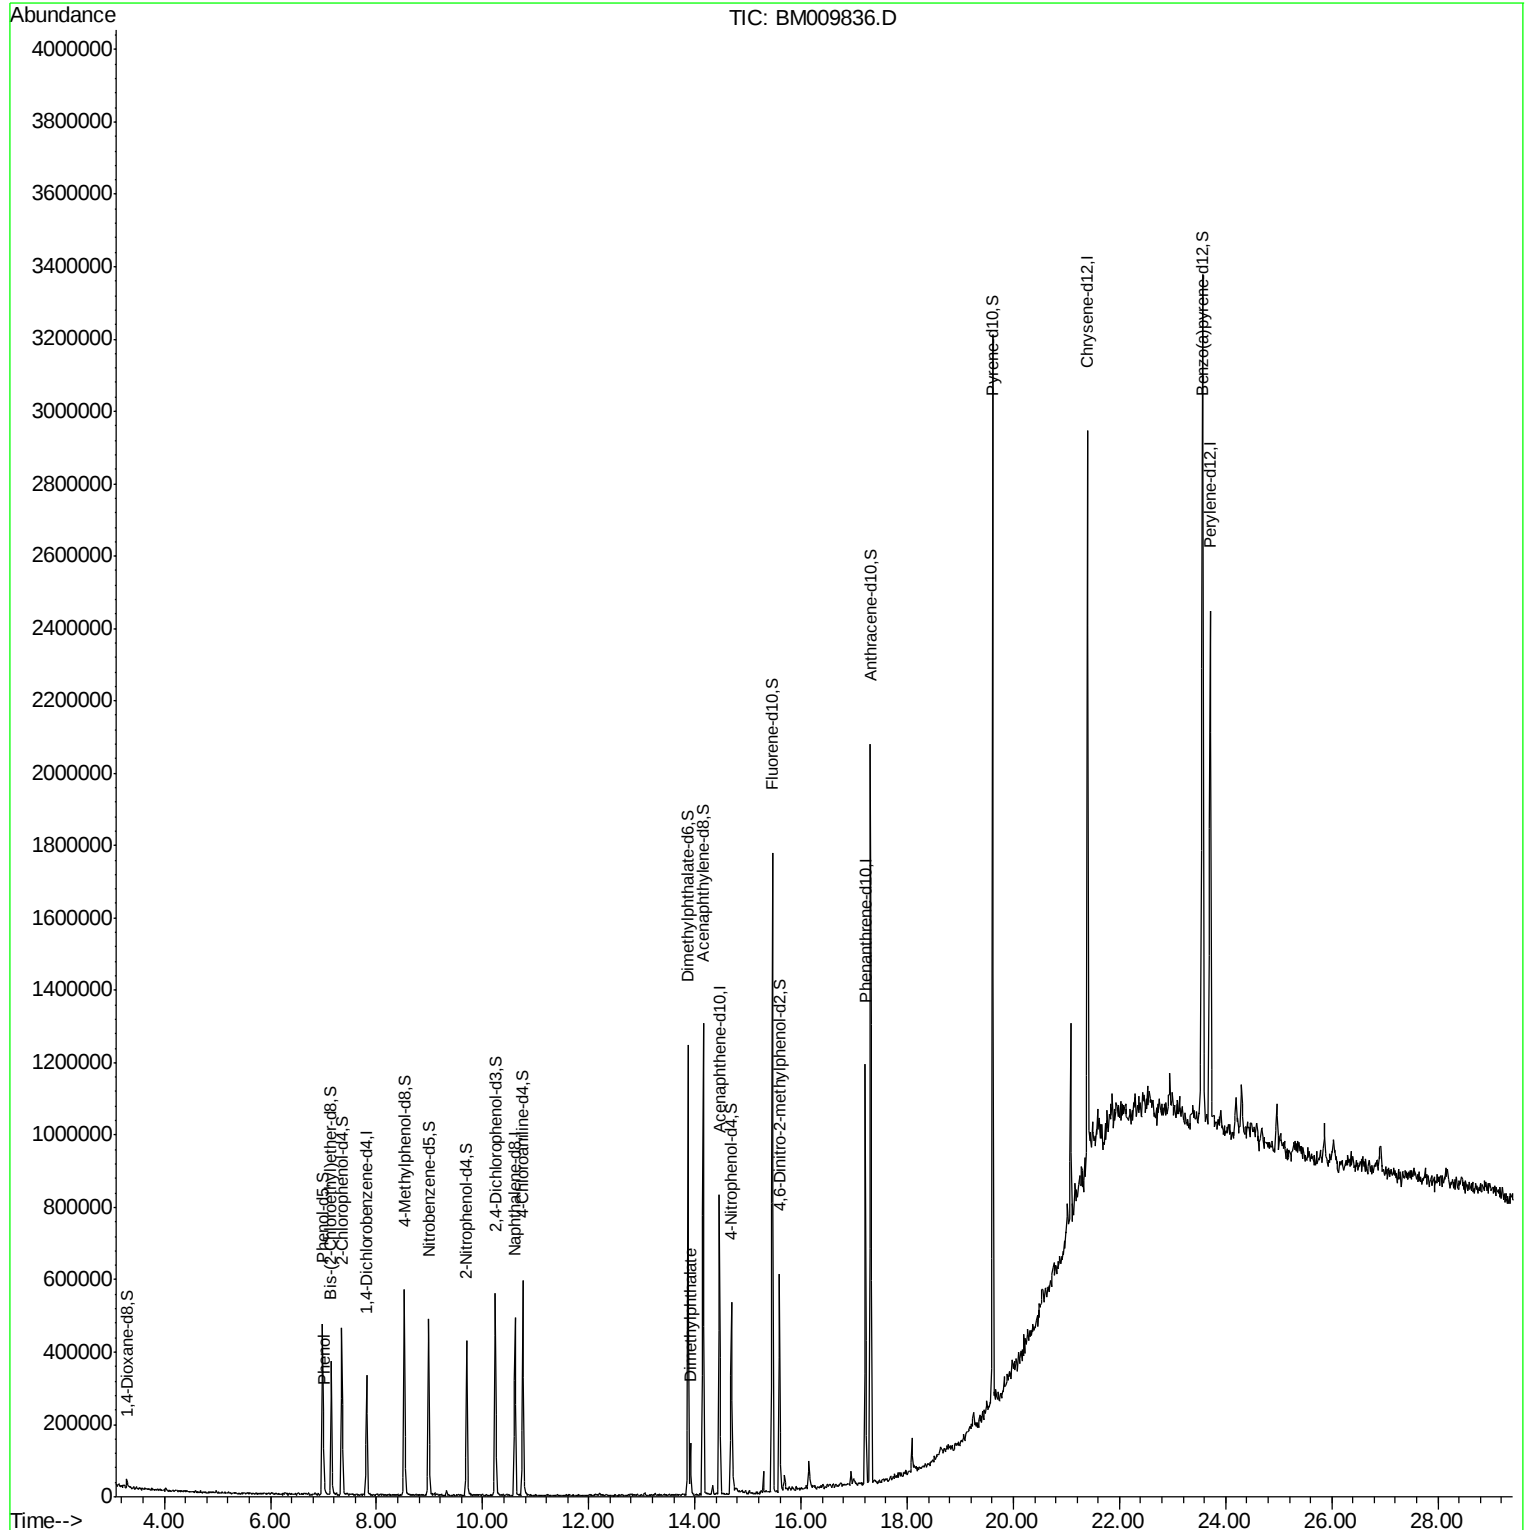

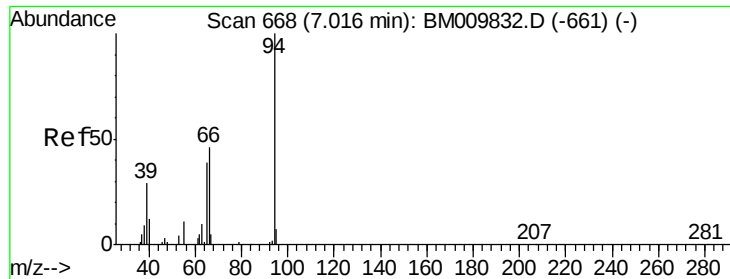

#6

Phenol

Concen: 1.99 ng/ul

RT: 7.01 min Scan# 667

Delta R.T. -0.01 min

Lab File: BM009836.D

Acq: 01 May 2017 18:44

Instrument :

BNA_M

ClientSampleId :

JHT06


Tgt Ion: 94 Resp: 16437

Ion Ratio Lower Upper

94 100

65 32.6 39.8 59.6#




66 47.2 69.9 104.9#

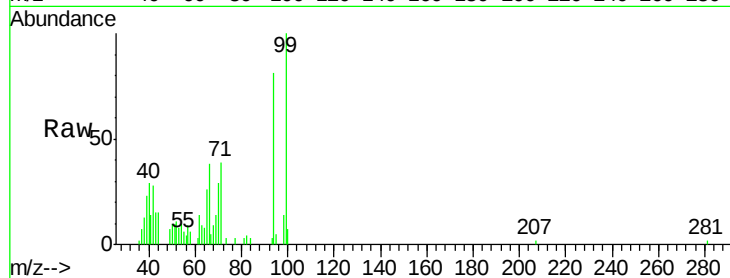

Abundance Ion 94.00 (93.70 to 94.70): BM009832.D (-661) (-)

Ion 65.00 (64.70 to 65.70): BM009832.D (-661) (-)

Ion 66.00 (65.70 to 66.70): BM009832.D (-661) (-)

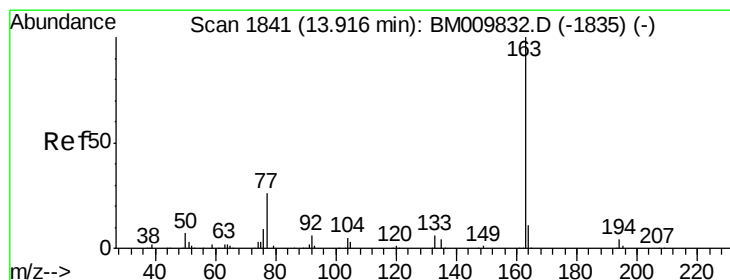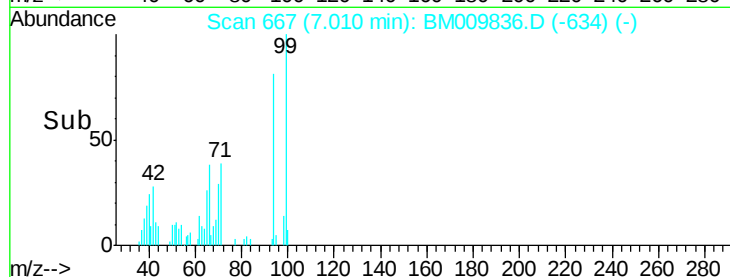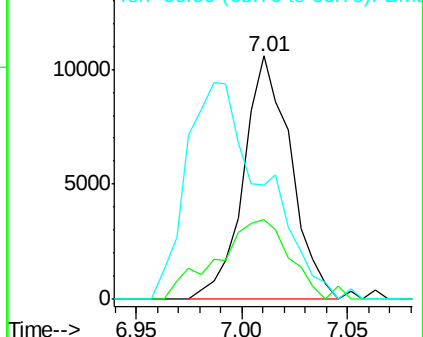

#44

Dimethylphthalate

Concen: 3.36 ng/ul

RT: 13.92 min Scan# 1841

Delta R.T. -0.00 min

Lab File: BM009836.D

Acq: 01 May 2017 18:44


Tgt Ion: 163 Resp: 70118

Ion Ratio Lower Upper

163 100

194 4.4 3.0 4.6

164 11.7 8.6 12.8

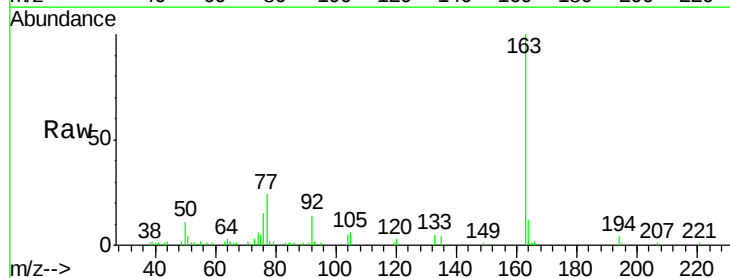

Abundance Ion 163.00 (162.70 to 163.70): BM009832.D (-1835) (-)

Ion 194.00 (193.70 to 194.70): BM009832.D (-1835) (-)

Ion 164.00 (163.70 to 164.70): BM009832.D (-1835) (-)

