

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050117\
 Data File : BM009861.D
 Acq On : 02 May 2017 09:49
 Operator : SJ/MA
 Sample : I2848-02DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHT04DL

Quant Time: May 02 13:57:28 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 02 01:45:45 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	115213	20.00	ng/ul	0.01
18) Naphthalene-d8	10.63	136	517180	20.00	ng/ul	0.02
35) Acenaphthene-d10	14.48	164	301282	20.00	ng/ul	0.02
61) Phenanthrene-d10	17.23	188	715047	20.00	ng/ul	0.02
75) Chrysene-d12	21.42	240	713360	20.00	ng/ul	0.02
83) Perylene-d12	23.74	264	678883	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	2893	1.16	ng/uL	0.01
5) Phenol-d5	7.02	99	41759	3.34	ng/ul	0.04
7) Bis-(2-Chloroethyl)ether-d	7.16	67	31491	3.69	ng/ul	0.01
9) 2-Chlorophenol-d4	7.36	132	32160	4.04	ng/ul	0.02
13) 4-Methylphenol-d8	8.56	113	32310	3.31	ng/ul	0.04
19) Nitrobenzene-d5	9.00	128	15219	3.62	ng/ul	0.02
22) 2-Nitrophenol-d4	9.72	143	15052	3.40	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	10.27	165	30189	3.41	ng/ul	0.04
29) 4-Chloroaniline-d4	10.78	131	36139	3.39	ng/ul	0.02
43) Dimethylphthalate-d6	13.88	166	104748	4.00	ng/ul	0.01
46) Acenaphthylene-d8	14.17	160	124472	3.94	ng/ul	0.02
51) 4-Nitrophenol-d4	14.75	143	10966	2.17	ng/ul	0.07
57) Fluorene-d10	15.47	176	95173	4.02	ng/ul	0.02
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.33	188	153672	4.19	ng/ul	0.02
76) Pyrene-d10	19.63	212	156019	4.96	ng/ul	0.02
87) Benzo(a)pyrene-d12	23.59	264	128600	3.89	ng/ul	0.03


Target Compounds					Qvalue
81) Bis(2-ethylhexyl)phthalate	21.30	149	625505	24.71 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050117\
Data File : BM009861.D
Acq On : 02 May 2017 09:49
Operator : SJ/MA
Sample : I2848-02DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT04DL

Quant Time: May 02 13:57:28 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 02 01:45:45 2017
Response via : Initial Calibration

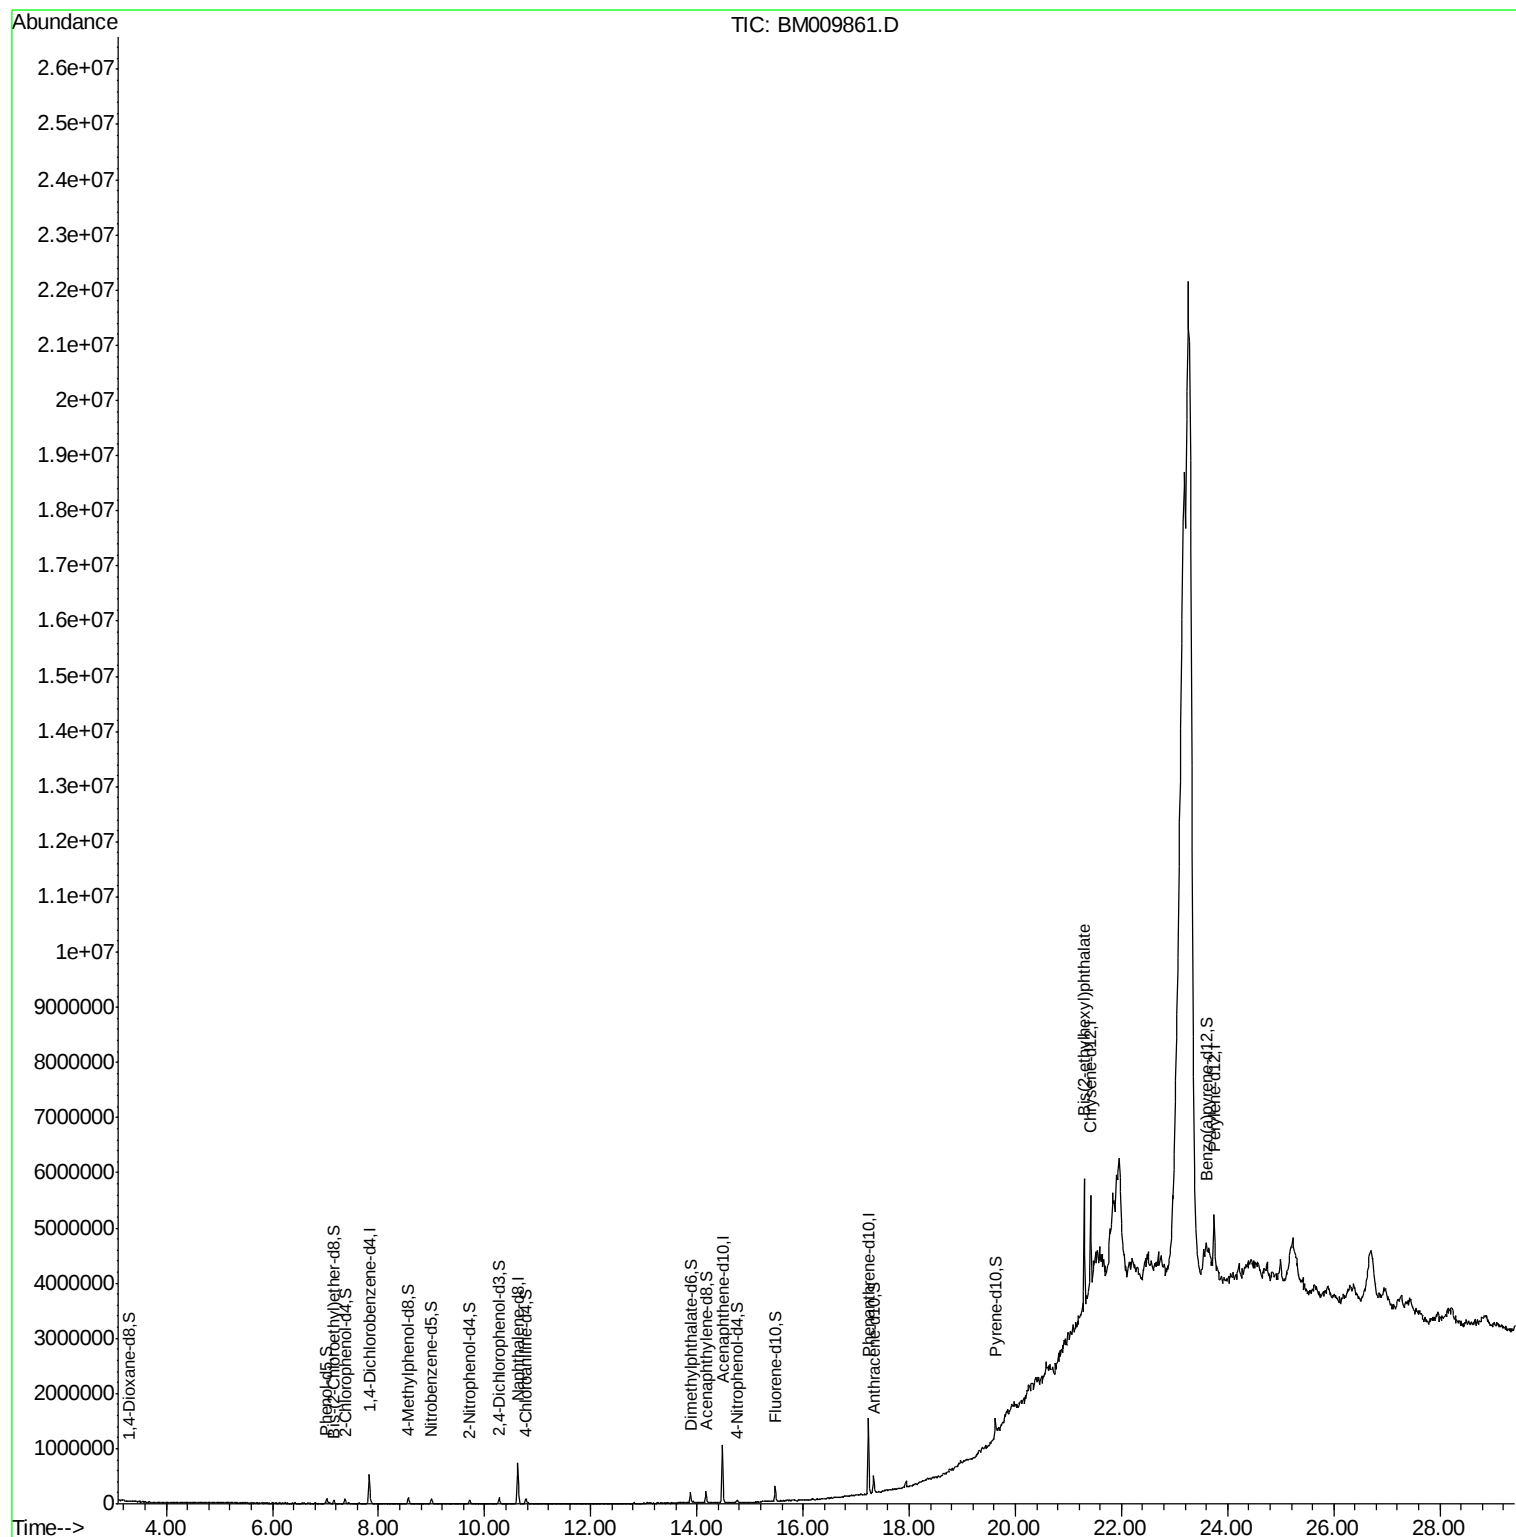

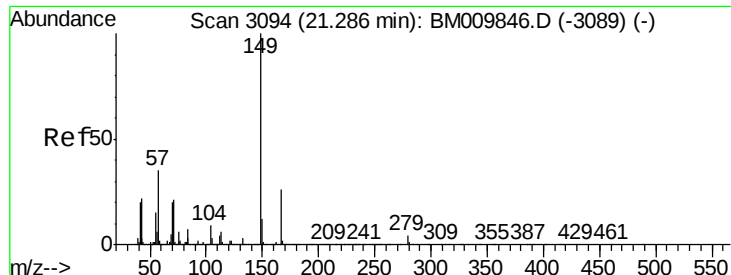

#81

Bis(2-ethylhexyl)phthalate

Concen: 24.71 ng/ul

RT: 21.30 min Scan# 3096

Delta R.T. 0.01 min

Lab File: BM009861.D

Acq: 02 May 2017 09:49

Instrument :

BNA_M

ClientSampleId :

JHT04DL

Tgt Ion:149 Resp: 625505

Ion Ratio Lower Upper

149 100

167 26.0 20.2 30.2

279 4.8 4.0 6.0

