

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050118\
 Data File : BM014889.D
 Acq On : 01 May 2018 17:12
 Operator : SJ/JU
 Sample : PB108678BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 02 04:56:42 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 04:52:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	334076	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1359019	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	674740	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1345514	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1263334	20.00	ng/ul	0.00
83) Perylene-d12	24.39	264	1320410	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.64	96	54552	7.13	ng/uL	0.00
5) Phenol-d5	7.62	99	895339	34.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	613055	37.02	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	747648	34.61	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	693721	33.68	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	334853	34.08	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	346622	35.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	621437	31.26	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	944017	48.11	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	1904312	36.16	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2204056	33.89	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	304137	31.11	ng/ul	0.00
57) Fluorene-d10	16.08	176	1581729	34.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	191555	26.31	ng/ul	0.00
70) Anthracene-d10	17.91	188	2346584	37.42	ng/ul	0.00
76) Pyrene-d10	20.15	212	2356424	39.42	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.23	264	2585444	39.85	ng/ul	0.00
Target Compounds						
15) N-Nitroso-di-n-propylamine	9.19	70	17616	1.125	ng/ul#	1
45) 2,6-Dinitrotoluene	14.49	165	13206	1.414	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050118\
Data File : BM014889.D
Acq On : 01 May 2018 17:12
Operator : SJ/JU
Sample : PB108678BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 02 04:56:42 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 04:52:22 2018
Response via : Initial Calibration

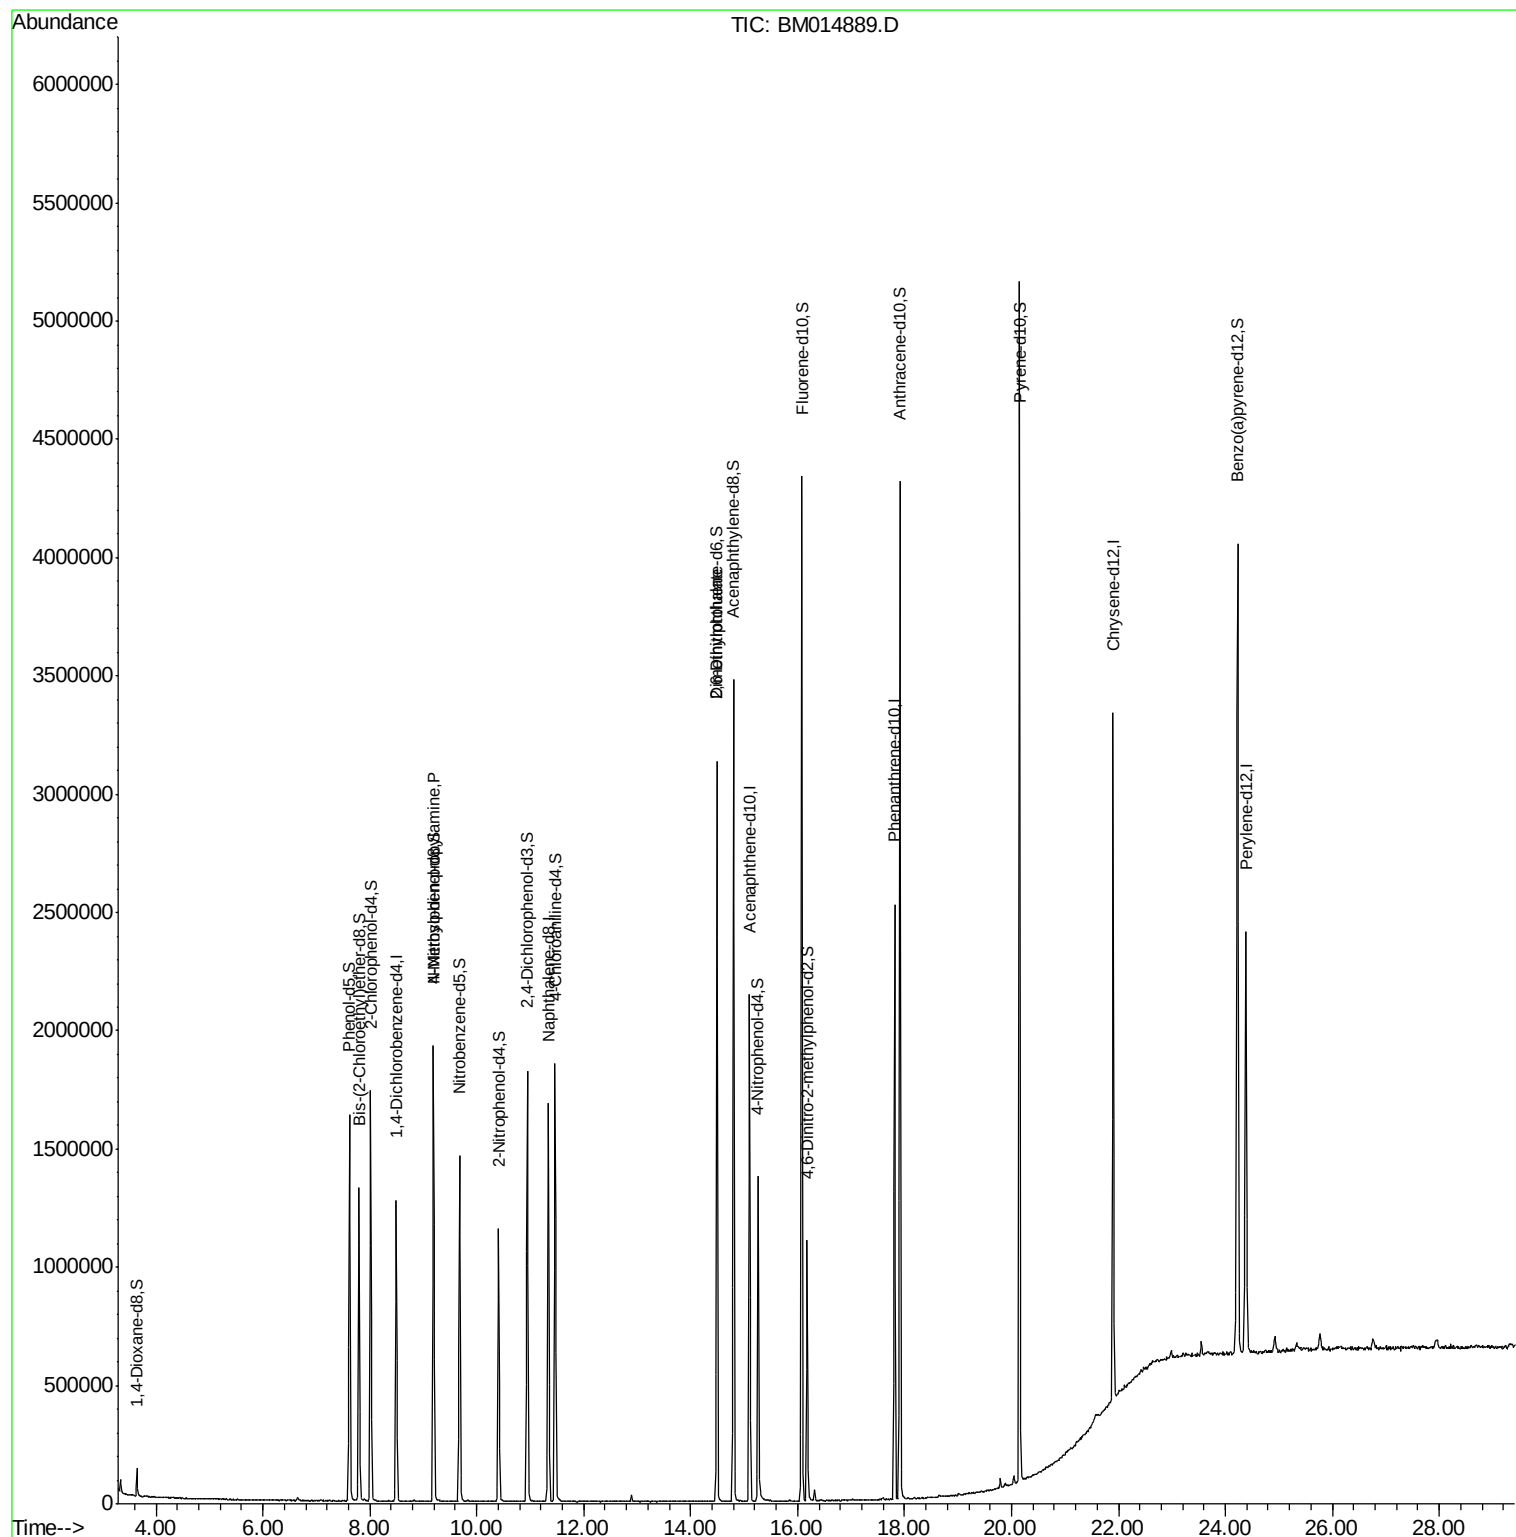

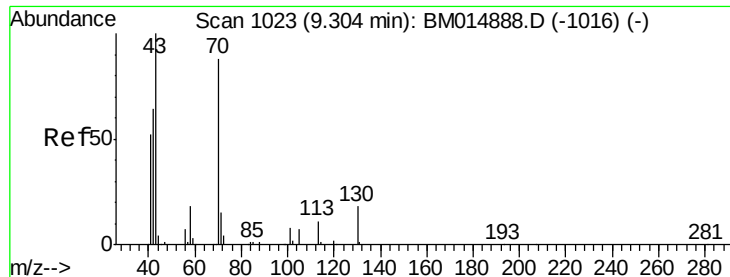

#15

N-Nitroso-di-n-propylamine

Concen: 1.125 ng/ul

RT: 9.19 min Scan# 1004

Delta R.T. -0.11 min

Lab File: BM014889.D

Acq: 01 May 2018 17:12

Instrument :

BNA_M

ClientSampleId :

Tot Ion: 70 Resp: 17616


Ion Ratio Lower Upper

70 100

42 455.3 76.0 114.0#

101 0.0 6.7 10.1#

130 0.0 14.6 22.0#

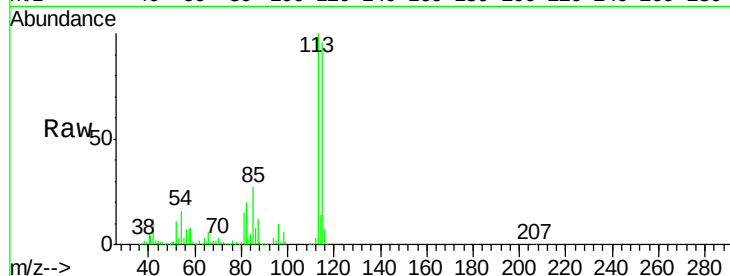




Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

Time-->

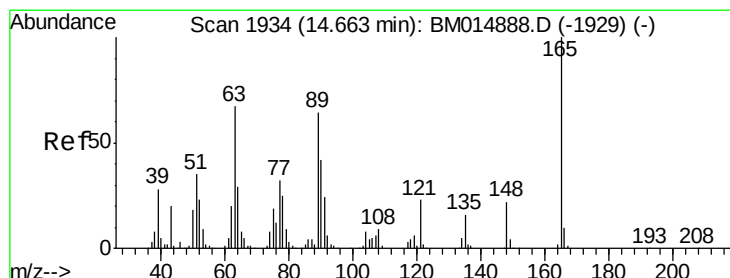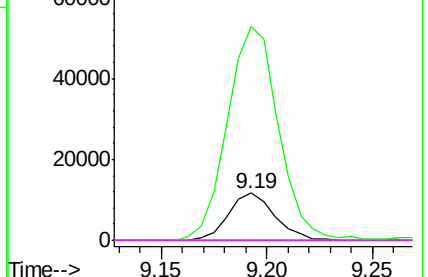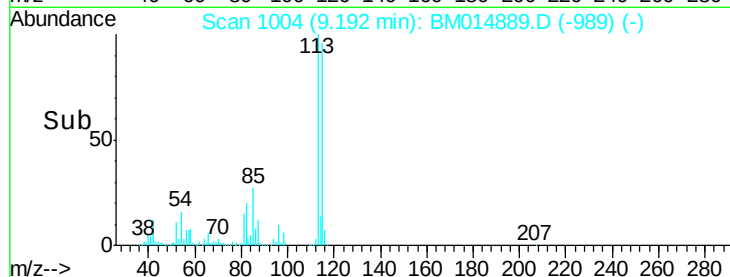

#45

2,6-Dinitrotoluene

Concen: 1.414 ng/ul

RT: 14.49 min Scan# 1905

Delta R.T. -0.17 min

Lab File: BM014889.D

Acq: 01 May 2018 17:12


Tgt Ion: 165 Resp: 13206

Ion Ratio Lower Upper

165 100

89 0.0 52.6 79.0#

121 36.5 14.6 22.0#

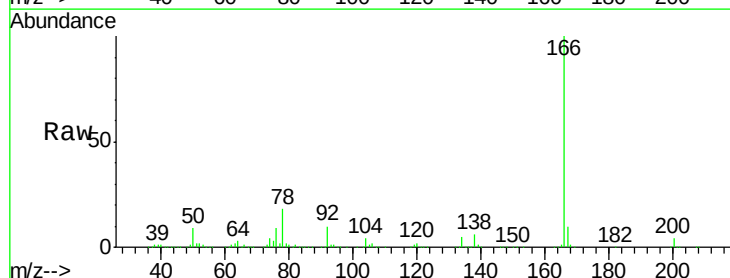

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

Time-->

