

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050118\
 Data File : BM014895.D
 Acq On : 01 May 2018 20:54
 Operator : SJ/JU
 Sample : J2636-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 02 04:58:16 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 04:52:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	386609	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1643916	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	855706	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1791004	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1669262	20.00	ng/ul	0.00
83) Perylene-d12	24.39	264	1613980	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	66159	7.47	ng/uL	0.00
5) Phenol-d5	7.62	99	251841	8.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	738150	38.51	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	744386	29.77	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	461793	19.38	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	421501	35.46	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	441347	37.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	745008	30.98	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	2982	0.13	ng/ul	0.01
43) Dimethylphthalate-d6	14.49	166	2428485	36.36	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2811100	34.08	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	74075	5.98	ng/ul	0.00
57) Fluorene-d10	16.08	176	2033932	35.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	291149	30.04	ng/ul	0.00
70) Anthracene-d10	17.92	188	3028398	36.28	ng/ul	0.00
76) Pyrene-d10	20.15	212	3115621	39.45	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.23	264	3090578	38.98	ng/ul	0.00


Target Compounds				Ovalue	
45) 2,6-Dinitrotoluene	14.50	165	16408	1.385	ng/ul# 28




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050118\
Data File : BM014895.D
Acq On : 01 May 2018 20:54
Operator : SJ/JU
Sample : J2636-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 02 04:58:16 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 04:52:22 2018
Response via : Initial Calibration

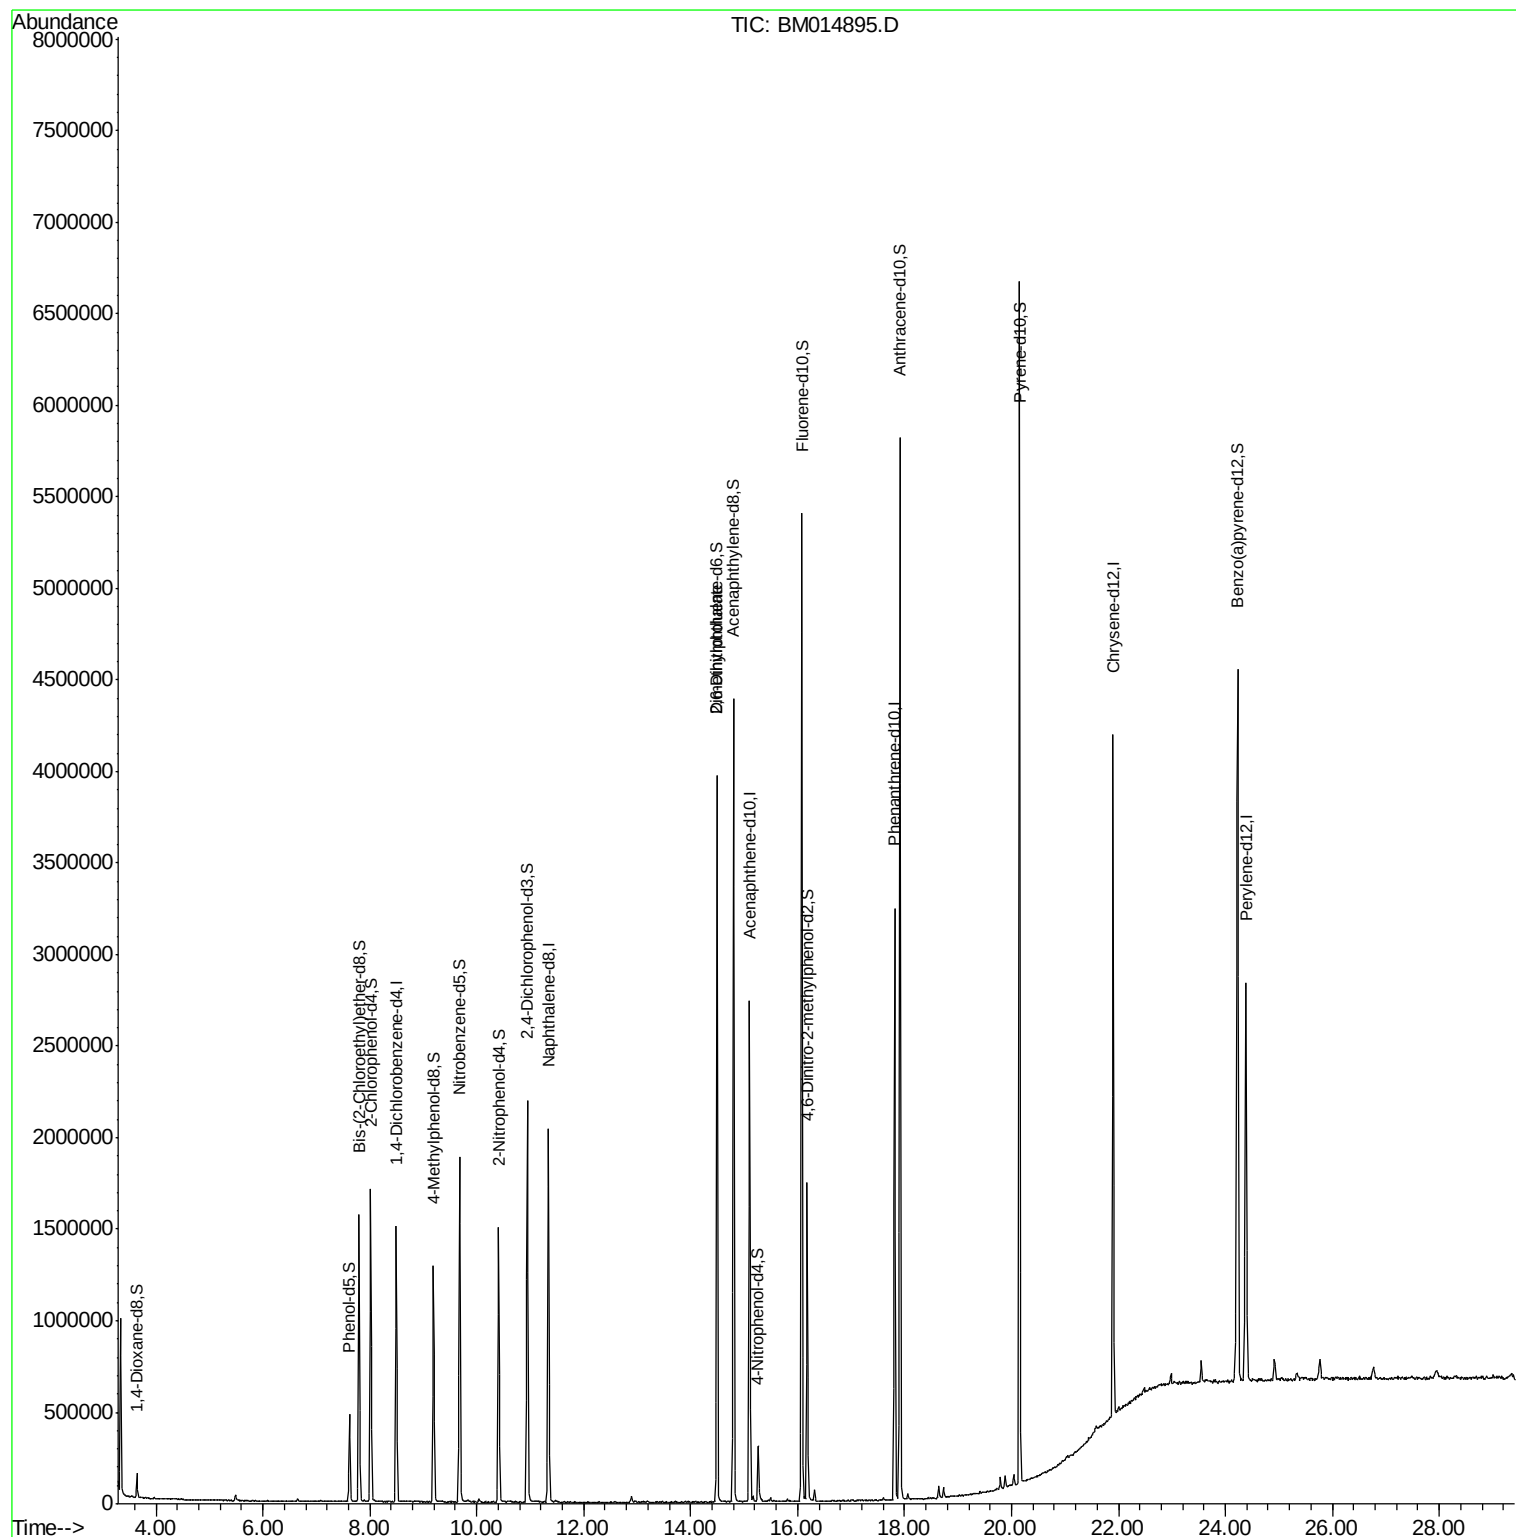

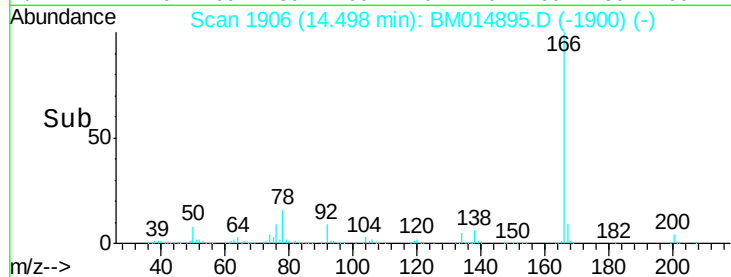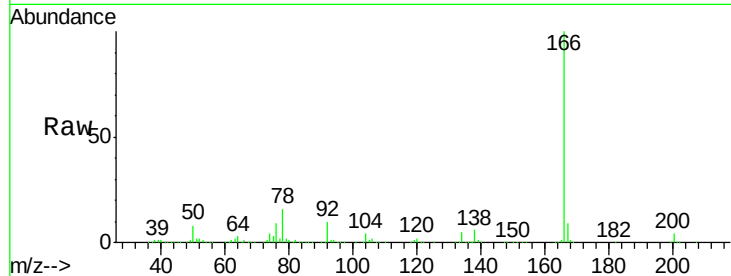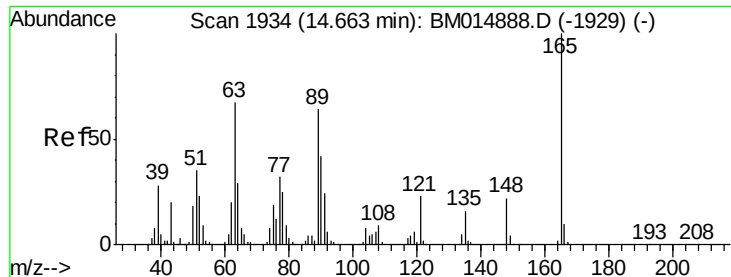

#45
 2,6-Dinitrotoluene
 Concen: 1.385 ng/ul
 RT: 14.50 min Scan# 1906
 Delta R.T. -0.16 min
 Lab File: BM014895.D
 Acq: 01 May 2018 20:54

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.6	79.0
121	32.3	14.6	22.0

