

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050118\
 Data File : BM014898.D
 Acq On : 01 May 2018 22:45
 Operator : SJ/JU
 Sample : J2638-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 02 04:58:56 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 04:52:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	400788	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1690070	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	865275	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1708610	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1526787	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1545179	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	65519	7.14	ng/uL	0.00
5) Phenol-d5	7.62	99	229782	7.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	722174	36.35	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	709831	27.39	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	413006	16.72	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	410285	33.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	427849	35.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	719806	29.12	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	29121	1.19	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	2271594	33.63	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2690478	32.26	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	57706	4.60	ng/ul	0.00
57) Fluorene-d10	16.08	176	1896401	32.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	258895	28.00	ng/ul	0.00
70) Anthracene-d10	17.91	188	2777766	34.89	ng/ul	0.00
76) Pyrene-d10	20.15	212	2755111	38.14	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	2839346	37.40	ng/ul	0.00

Target Compounds


				Ovalue		
6) Phenol	7.65	94	36377	1.193	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050118\
Data File : BM014898.D
Acq On : 01 May 2018 22:45
Operator : SJ/JU
Sample : J2638-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 02 04:58:56 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 04:52:22 2018
Response via : Initial Calibration

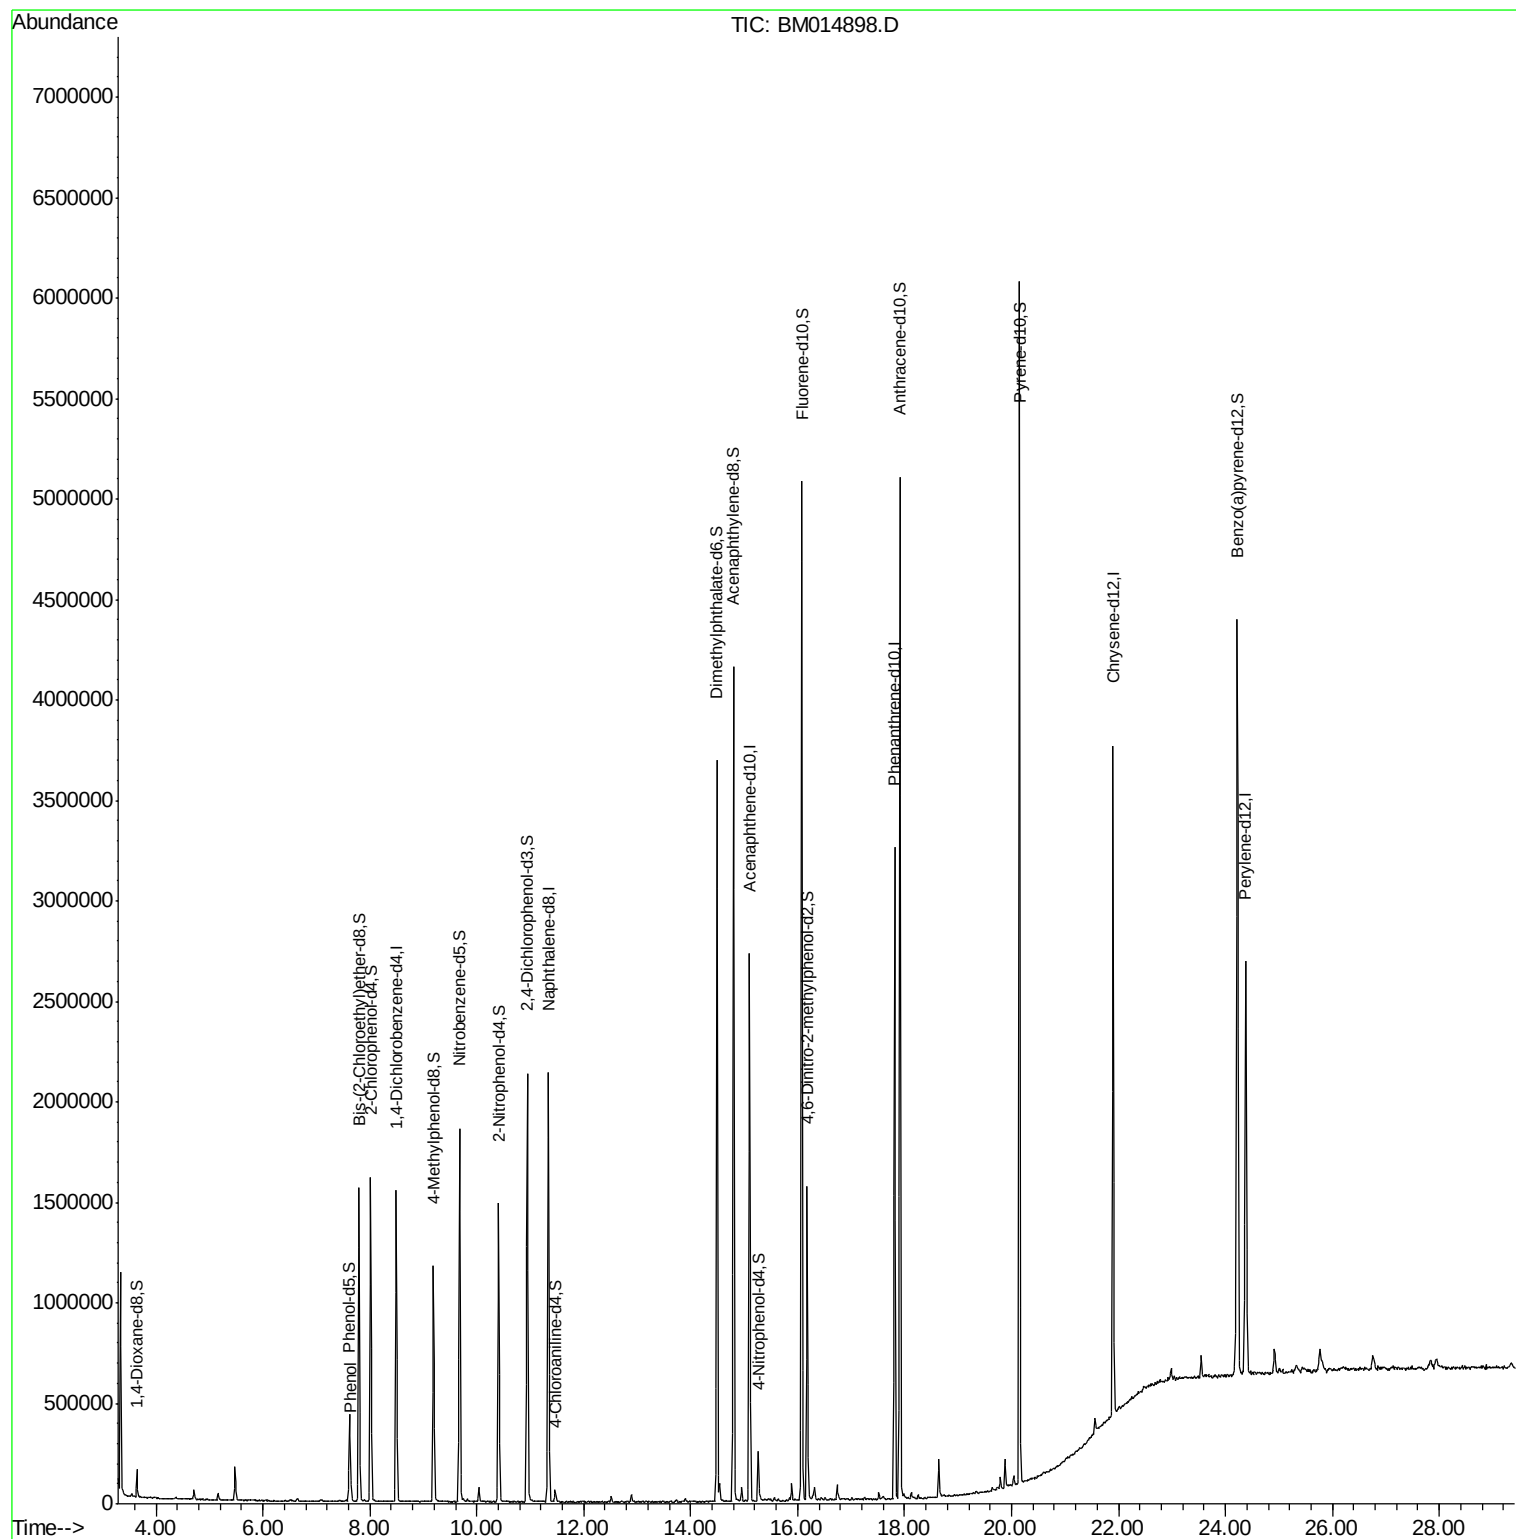

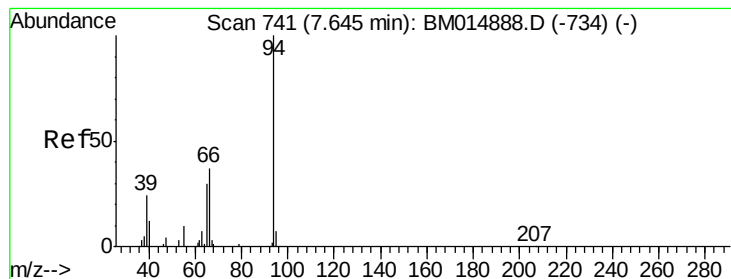


#6

Phenol

Concen: 1.193 ng/ul
 RT: 7.65 min Scan# 741
 Delta R.T. -0.00 min
 Lab File: BM014898.D
 Acq: 01 May 2018 22:45

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
94	100		
65	33.1	28.2	42.4
66	40.3	47.2	70.8

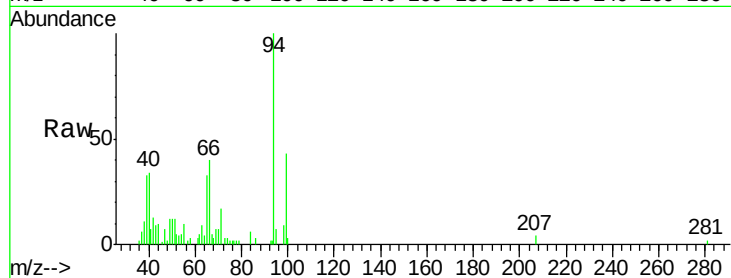

Abundance

Ion 94.00 (93.70 to 94.70): BM014898.D (-707) (-)

Ion 65.00 (64.70 to 65.70): BM014898.D (-707) (-)

Ion 66.00 (65.70 to 66.70): BM014898.D (-707) (-)

