

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
 Data File : BM014900.D
 Acq On : 01 May 2018 23:59
 Operator : SJ/JU
 Sample : J2638-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA1

Quant Time: May 02 04:59:21 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 04:52:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	377315	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1591389	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	827540	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1740607	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1649097	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1588591	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.64	96	65709	7.60	ng/uL	0.00
5) Phenol-d5	7.62	99	237368	8.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	748197	40.00	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	734780	30.11	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	434882	18.70	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	430848	37.45	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	450361	39.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	749792	32.21	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	10002	0.44	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	2451470	37.95	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2884476	36.16	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	66623	5.56	ng/ul	0.00
57) Fluorene-d10	16.08	176	2058964	36.65	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	297810	31.62	ng/ul	0.00
70) Anthracene-d10	17.91	188	3081270	37.99	ng/ul	0.00
76) Pyrene-d10	20.15	212	3203883	41.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	3175199	40.68	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.54	163	97705	1.565	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
Data File : BM014900.D
Acq On : 01 May 2018 23:59
Operator : SJ/JU
Sample : J2638-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA1

Quant Time: May 02 04:59:21 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 04:52:22 2018
Response via : Initial Calibration

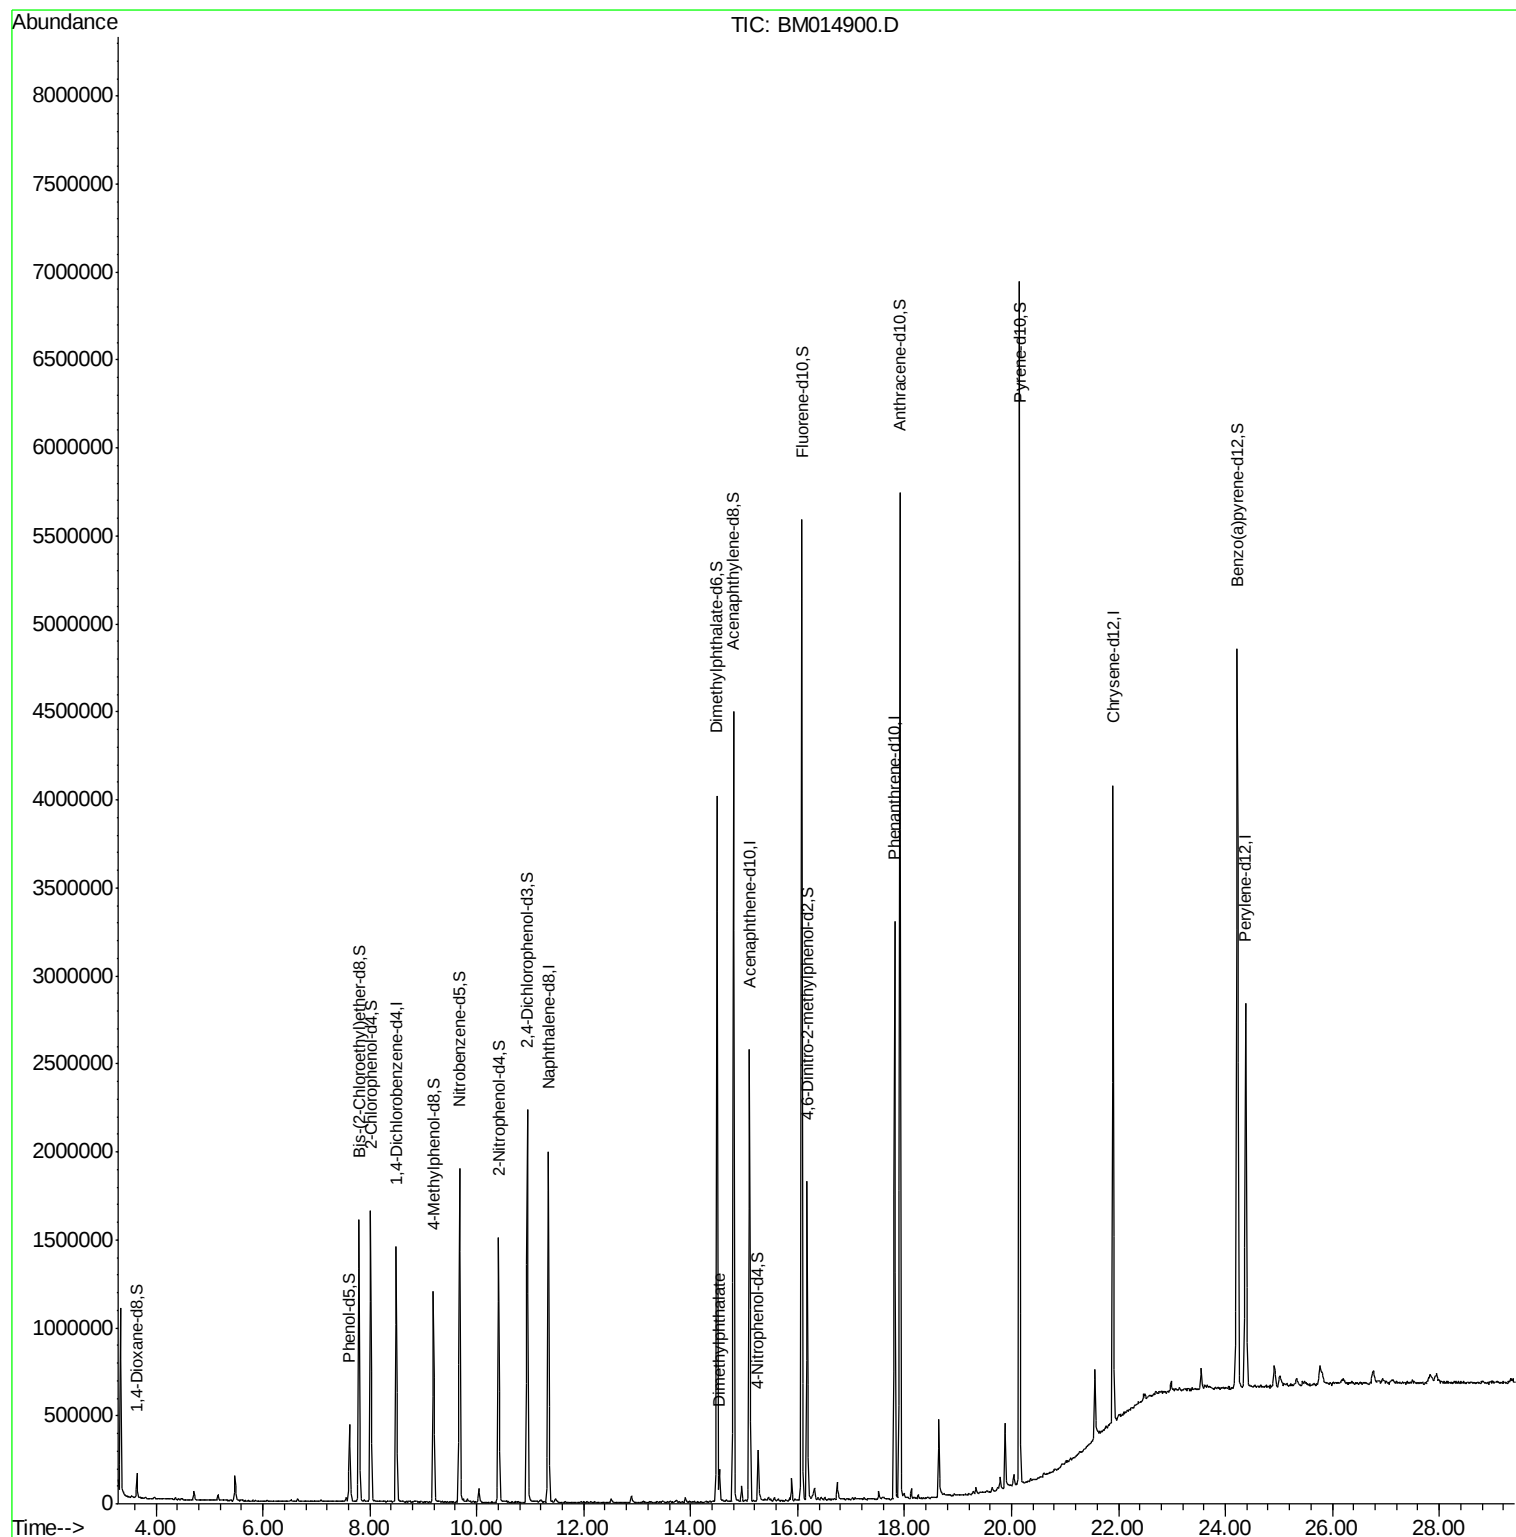

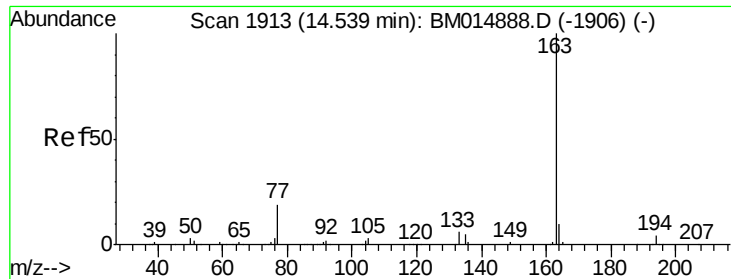

#44
 Dimethylphthalate
 Concen: 1.565 ng/ul
 RT: 14.54 min Scan# 1913
 Delta R.T. 0.00 min
 Lab File: BM014900.D
 Acq: 01 May 2018 23:59

Instrument :
 BNA_M
 ClientSampleId :
 C0AA1

Tgt Ion:163 Resp: 97705
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.5 5.3
 164 9.6 8.2 12.4

