

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
 Data File : BM014902.D
 Acq On : 02 May 2018 01:13
 Operator : SJ/JU
 Sample : J2638-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA6

Quant Time: May 02 04:59:46 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 04:52:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	417631	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1785053	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	945130	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	2004654	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1893281	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1731433	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	71521	7.48	ng/uL	0.00
5) Phenol-d5	7.62	99	291735	9.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	811252	39.18	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	829269	30.70	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	505303	19.63	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	469149	36.35	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	485131	37.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	829904	31.78	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	44044	1.71	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	2686100	36.41	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	3136381	34.43	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	85474	6.24	ng/ul	0.00
57) Fluorene-d10	16.08	176	2239096	34.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	332396	30.64	ng/ul	0.00
70) Anthracene-d10	17.92	188	3343620	35.79	ng/ul	0.00
76) Pyrene-d10	20.15	212	3476623	38.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	3288215	38.66	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.54	163	193314	2.711	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
Data File : BM014902.D
Acq On : 02 May 2018 01:13
Operator : SJ/JU
Sample : J2638-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA6

Quant Time: May 02 04:59:46 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 04:52:22 2018
Response via : Initial Calibration

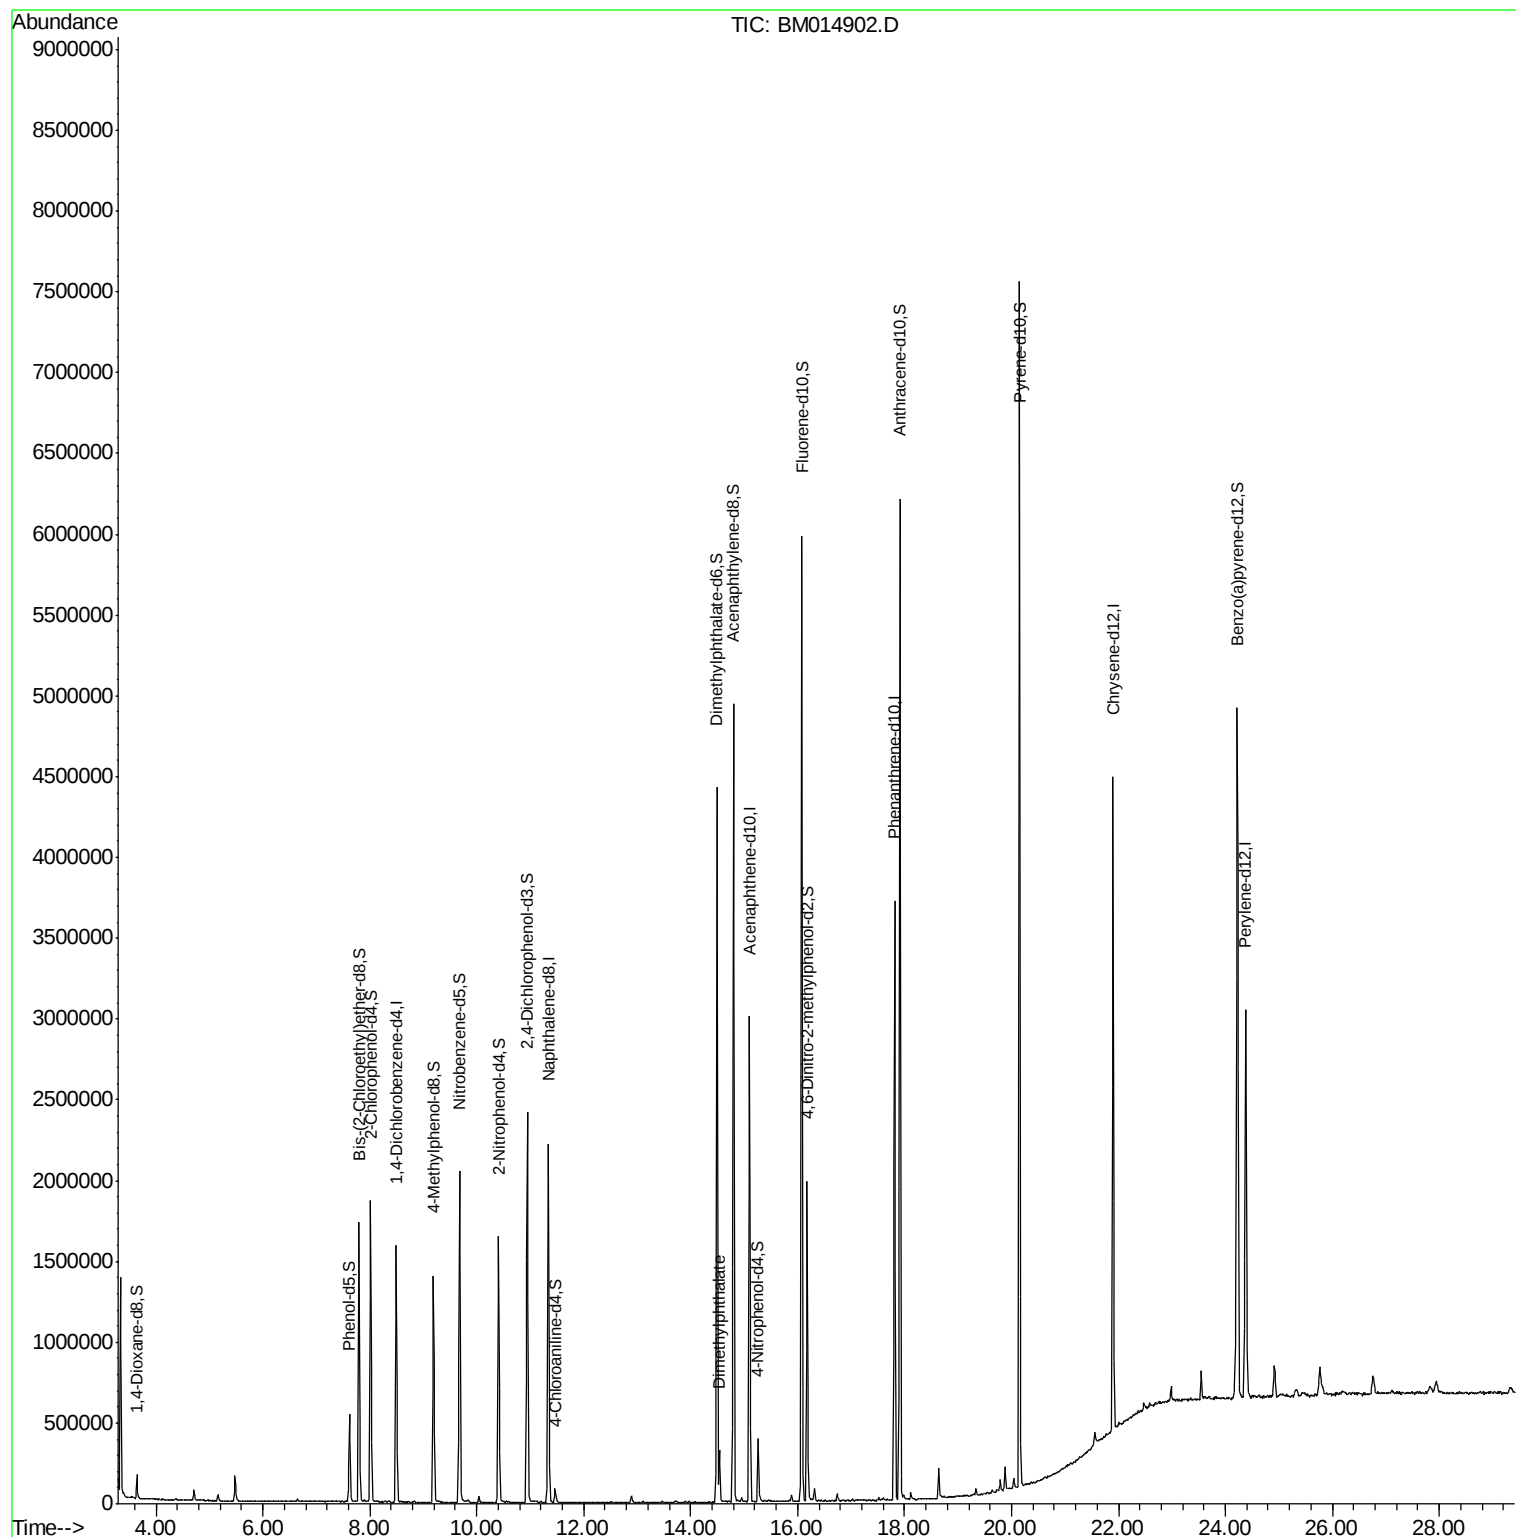

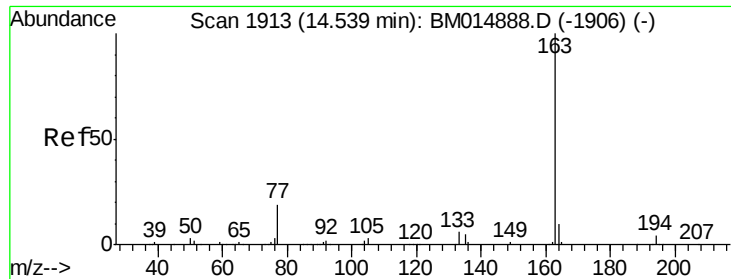

#44

Dimethylphthalate

Concen: 2.711 ng/ul

RT: 14.54 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BM014902.D

Acq: 02 May 2018 01:13

Instrument :

BNA_M

ClientSampleId :

C0AA6


Tgt Ion:163 Resp: 193314

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.9 8.2 12.4

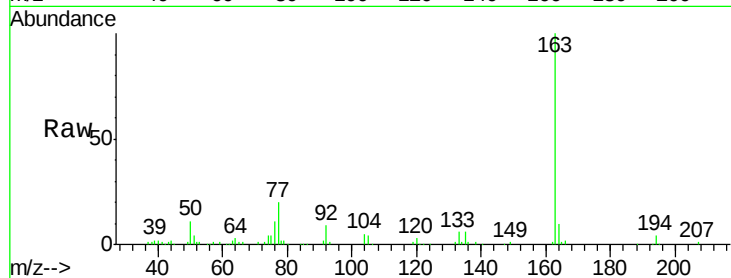

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

